

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\UStol-5_P1-C-6_01_8132.d
Method lc_qtof_directospos.m
Sample Name UStol-5
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 3:59:49 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

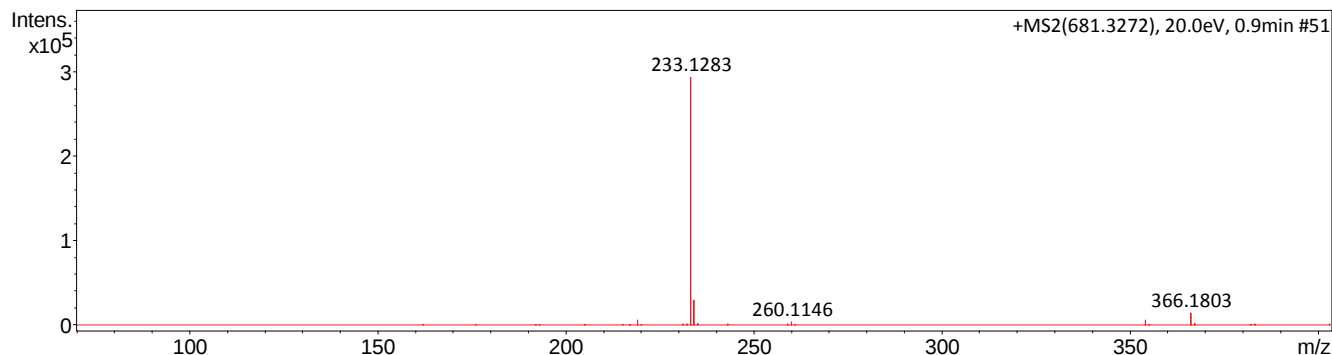

#	m/z	I	I %
1	162.0871	904	0.3
2	176.1044	992	0.3
3	192.0878	791	0.3
4	193.0968	1291	0.4
5	205.1252	864	0.3
6	215.1164	723	0.2
7	217.1003	735	0.3
8	219.1112	5964	2.0
9	220.0993	813	0.3
10	231.1115	1838	0.6
11	232.1183	1915	0.7
12	233.1283	292489	100.0
13	234.1304	29479	10.1
14	235.1347	2408	0.8
15	243.1108	1728	0.6
16	259.1061	2014	0.7
17	260.1146	4322	1.5
18	261.1170	1035	0.4
19	298.1414	481	0.2
20	354.1432	6464	2.2
21	355.1492	1039	0.4
22	366.1803	14493	5.0
23	367.1838	2531	0.9
24	382.1745	874	0.3
25	383.1825	2035	0.7
26	403.2006	1495	0.5
27	421.2105	566	0.2
28	530.2640	847	0.3
29	681.3272	1647	0.6
30	682.3250	431	0.1