

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\Gaby\Sabrina\MeOH NEG\D1 L Red Liofiliz_P1-D-4_01_4688.d
Method lcms2 esi neg ce20.m
Sample Name D1 L Red Liofiliz
Comment SV: DCM + MeOH
Rosana Misico


Acquisition Date 5/14/2022 1:45:44 AM

Operator GC
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	3.4 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

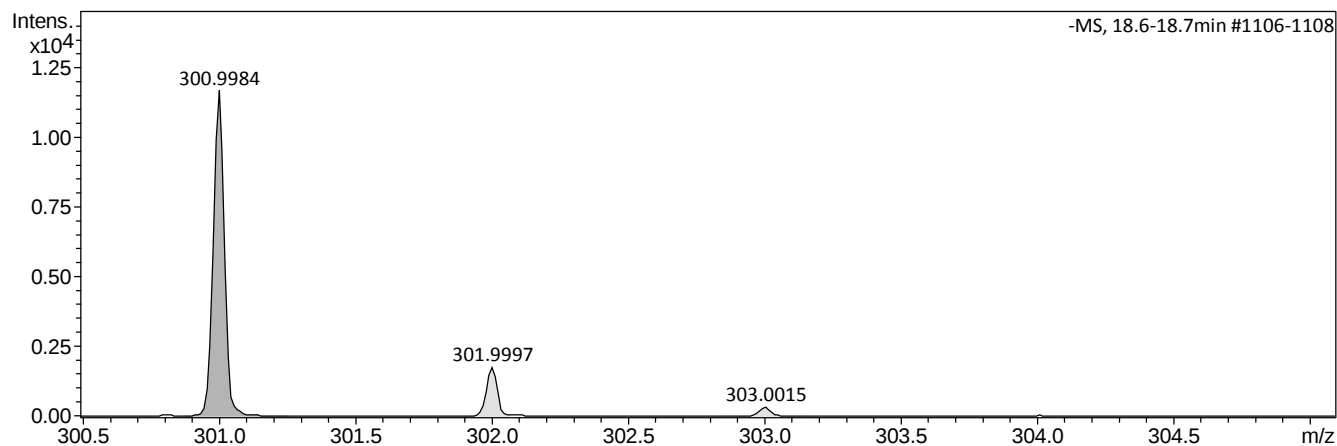

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
300.9984	1	C ₁₄ H ₅ O ₈	300.9990	2.1	3.2	1	100.00	12.5	even	ok