

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-112701_P1-D-1_01_10023.d
Method lc-ms auto pos batata 110225.m
Sample Name 24-112701
Comment Extracto cacao
Sv: MeOH
Ana Rojas
Depto. de Industrias / FCEN-UBA


Acquisition Date 2/11/2025 4:18:44 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.8 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1800 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

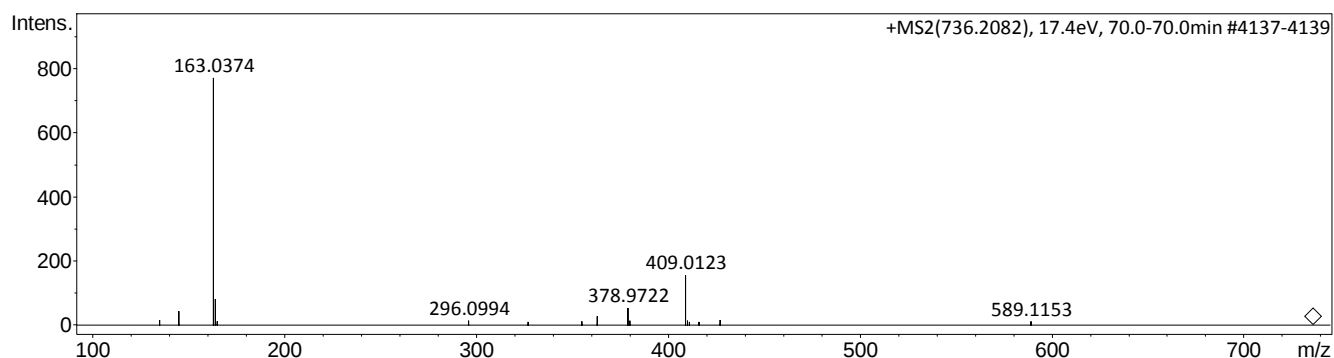

#	m/z	I	I %
1	135.0300	16	2.0
2	135.0434	13	1.7
3	145.0276	45	5.8
4	163.0374	769	100.0
5	164.0404	82	10.6
6	165.0384	12	1.6
7	296.0994	14	1.9
8	326.9763	11	1.4
9	355.0778	12	1.5
10	363.0026	27	3.6
11	378.9722	55	7.1
12	380.0048	14	1.9
13	409.0123	154	20.1
14	410.0351	14	1.9
15	411.0305	10	1.3
16	416.1524	10	1.3
17	427.0604	15	2.0
18	589.1153	12	1.6
19	761.0796	74	9.7
20	761.2485	21	2.7
21	761.4424	14	1.8
22	761.8246	10	1.3
23	763.1165	25	3.2
24	1074.3739	19	2.5
25	1441.5475	57	7.5