

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-112701_P1-D-1_01_10023.d
 Method lc-ms auto pos batata 110225.m
 Sample Name 24-112701
 Comment Extracto cacao
 Sv: MeOH
 Ana Rojas
 Depto. de Industrias / FCEN-UBA


Acquisition Date 2/11/2025 4:18:44 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.8 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1800 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

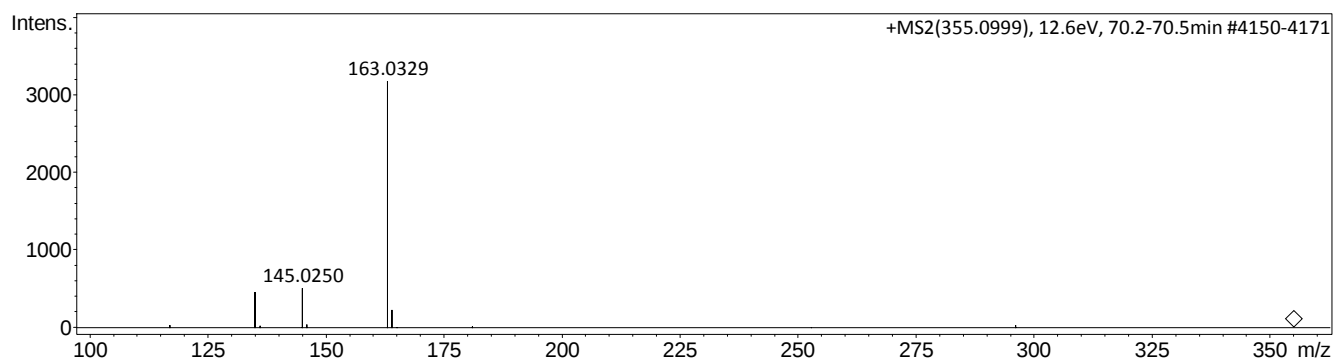

#	m/z	I	I %
1	89.0358	4	0.1
2	117.0269	26	0.8
3	135.0390	455	14.4
4	136.0424	22	0.7
5	145.0250	502	15.9
6	146.0268	41	1.3
7	163.0329	3169	100.0
8	164.0347	226	7.1
9	165.0406	4	0.1
10	181.0448	11	0.4
11	252.9715	3	0.1
12	296.0995	29	0.9
13	501.6554	16	0.5
14	761.0766	119	3.7
15	761.4451	16	0.5
16	761.5935	15	0.5
17	761.8202	11	0.4
18	761.9596	10	0.3
19	1074.3756	35	1.1
20	1251.2233	4	0.1
21	1441.5483	82	2.6
22	1442.7591	9	0.3