

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112701_P1-D-1_01_10023.d
Method lc-ms auto pos batata 110225.m
Sample Name 24-112701
Comment Extracto cacao
Sv: MeOH
Ana Rojas
Depto. de Industrias / FCEN-UBA

Acquisition Date 2/11/2025 4:18:44 PM

Operator EB - MV
Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.8 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1800 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

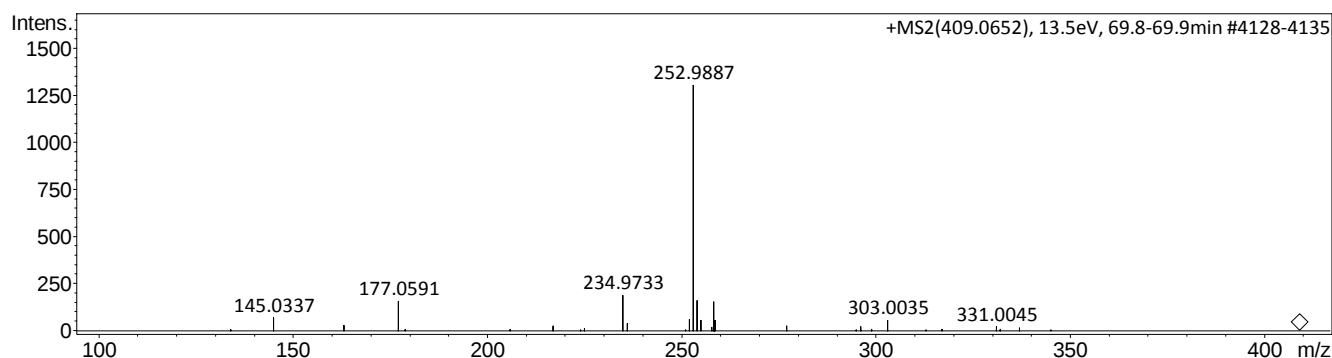

#	m/z	I	I %
1	134.0393	10	0.8
2	145.0337	72	5.5
3	163.0454	31	2.4
4	177.0591	157	12.1
5	216.9723	25	1.9
6	224.9913	13	1.0
7	234.9733	188	14.4
8	235.9814	38	2.9
9	251.9934	60	4.6
10	252.9887	1301	100.0
11	253.9909	161	12.4
12	254.9923	57	4.4
13	257.7706	21	1.6
14	258.3015	155	11.9
15	258.5346	23	1.8
16	258.6139	56	4.3
17	276.9988	25	1.9
18	296.1032	21	1.6
19	303.0035	55	4.2
20	331.0045	23	1.8
21	336.9890	15	1.2
22	501.6535	19	1.5
23	761.0778	122	9.4
24	761.5990	23	1.8
25	1074.3818	50	3.9
26	1357.3173	10	0.8
27	1441.5580	107	8.2
28	1442.0582	10	0.8
29	1442.2691	23	1.8
30	1442.7675	10	0.8