

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112701_P1-D-1_01_10023.d
Method lc-ms auto pos batata 110225.m
Sample Name 24-112701
Comment Extracto cacao
Sv: MeOH
Ana Rojas
Depto. de Industrias / FCEN-UBA

Acquisition Date 2/11/2025 4:18:44 PM

Operator EB - MV
Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.8 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1800 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

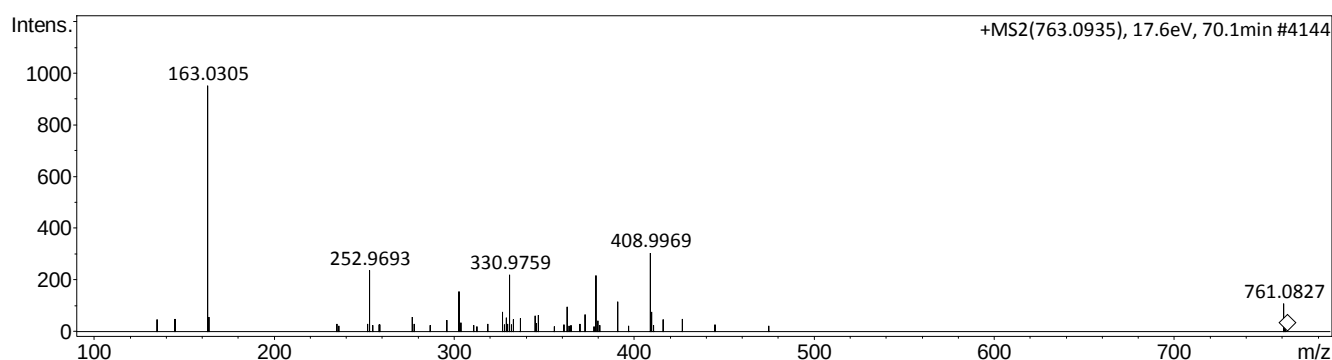

#	m/z	I	I %
1	135.0360	46	4.8
2	145.0181	50	5.3
3	163.0305	950	100.0
4	164.0315	58	6.1
5	234.9598	30	3.2
6	252.9693	237	24.9
7	276.9554	56	5.9
8	296.0986	45	4.7
9	302.9766	156	16.4
10	303.9939	34	3.6
11	326.9789	77	8.1
12	328.9869	54	5.7
13	330.9759	219	23.1
14	332.9900	48	5.1
15	336.9705	51	5.4
16	344.9907	62	6.5
17	345.9886	32	3.4
18	346.9725	64	6.7
19	362.9891	96	10.1
20	372.9838	66	6.9
21	378.9746	216	22.7
22	379.9848	42	4.4
23	390.9928	115	12.1
24	408.9969	304	32.0
25	410.0051	77	8.1
26	416.1490	48	5.1
27	427.0205	49	5.2
28	761.0827	108	11.4
29	761.4472	32	3.4
30	1441.5533	93	9.8