

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\24-112701_P1-D-1_01_10023.d
Method lc-ms auto pos batata 110225.m
Sample Name 24-112701
Comment Extracto cacao
Sv: MeOH
Ana Rojas
Depto. de Industrias / FCEN-UBA

Acquisition Date 2/11/2025 4:18:44 PM

Operator EB - MV
Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.8 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1800 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

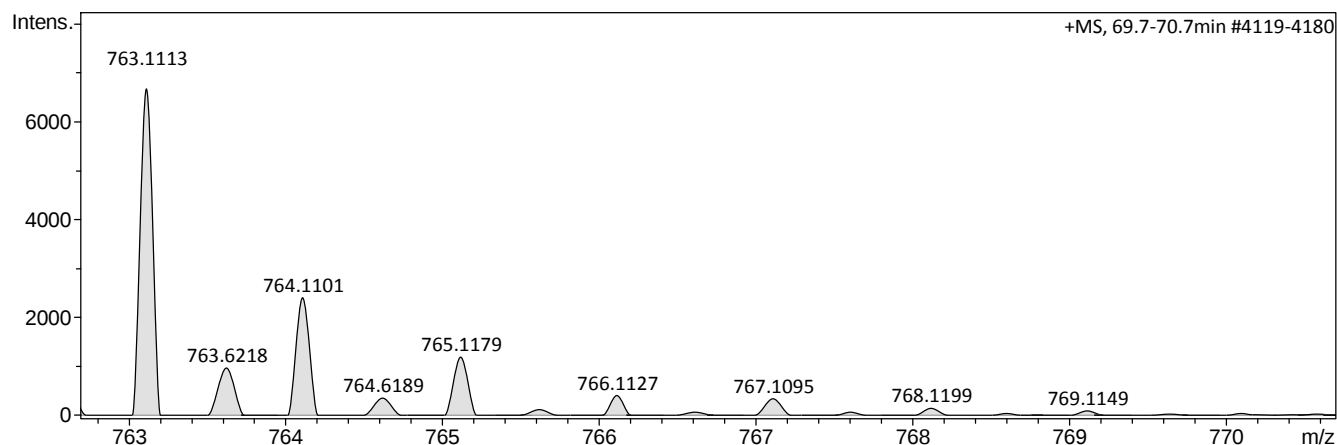

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
763.1113	1	C32H27O22	763.0988	-16.3	40.2	1	0.00	19.5	even	ok
	2	C36H27O19	763.1141	3.7	40.4	2	100.00	23.5	even	ok
	3	C29H31O24	763.1200	11.4	46.7	3	0.01	14.5	even	ok
	4	C39H23O17	763.0930	-24.0	46.9	4	0.00	28.5	even	ok
	5	C40H27O16	763.1294	23.7	50.4	5	0.00	27.5	even	ok
	6	C25H31O27	763.1047	-8.6	60.5	6	0.38	10.5	even	ok
	7	C43H23O14	763.1082	-4.0	61.5	7	44.03	32.5	even	ok
	8	C22H35O29	763.1259	19.1	72.9	8	0.00	5.5	even	ok
	9	C21H31O30	763.0895	-28.6	77.2	9	0.00	6.5	even	ok
	10	C47H23O11	763.1235	16.0	79.4	10	0.00	36.5	even	ok
	11	C18H35O32	763.1106	-0.9	90.7	11	79.80	1.5	even	ok