

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-120601_P1-B-5_01_9818.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-120601
 Comment SOL356
 Sv: DMSO + MeOH + HCOOH
 Mercedes Blanco

Acquisition Date 12/23/2024 12:20:19 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

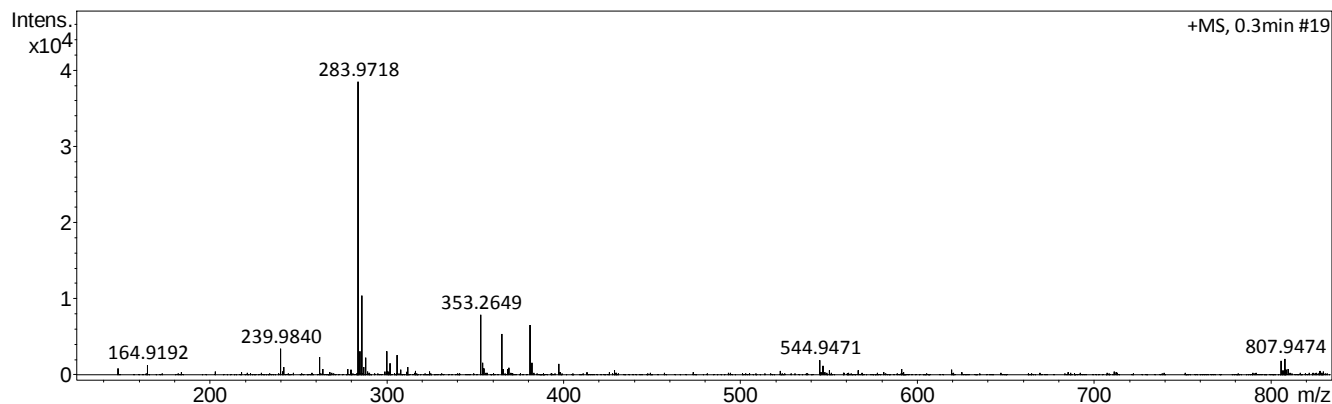

#	m/z	I	I %
1	148.1294	899	2.3
2	164.9192	1270	3.3
3	239.9840	3444	9.0
4	241.9814	1031	2.7
5	261.9865	2404	6.3
6	263.9843	802	2.1
7	277.9641	820	2.1
8	283.9718	38451	100.0
9	284.9759	3146	8.2
10	285.9675	10423	27.1
11	286.9705	1059	2.8
12	288.2920	2259	5.9
13	299.9434	3155	8.2
14	301.9429	1502	3.9
15	305.9488	2620	6.8
16	311.9547	1011	2.6
17	353.2649	7861	20.4
18	354.2672	1591	4.1
19	355.0688	838	2.2
20	365.1047	5403	14.1
21	369.2349	958	2.5
22	381.2939	6557	17.1
23	382.2953	1607	4.2
24	397.2680	1417	3.7
25	544.9471	1967	5.1
26	546.9457	1165	3.0
27	591.4922	795	2.1
28	805.9366	1873	4.9
29	807.9474	2088	5.4
30	809.9284	807	2.1