

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-120602_P1-B-6_01_9819.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-120602
 Comment SOL365
 Sv: DMSO + MeOH + HCOOH
 Mercedes Blanco

Acquisition Date 12/23/2024 12:25:26 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

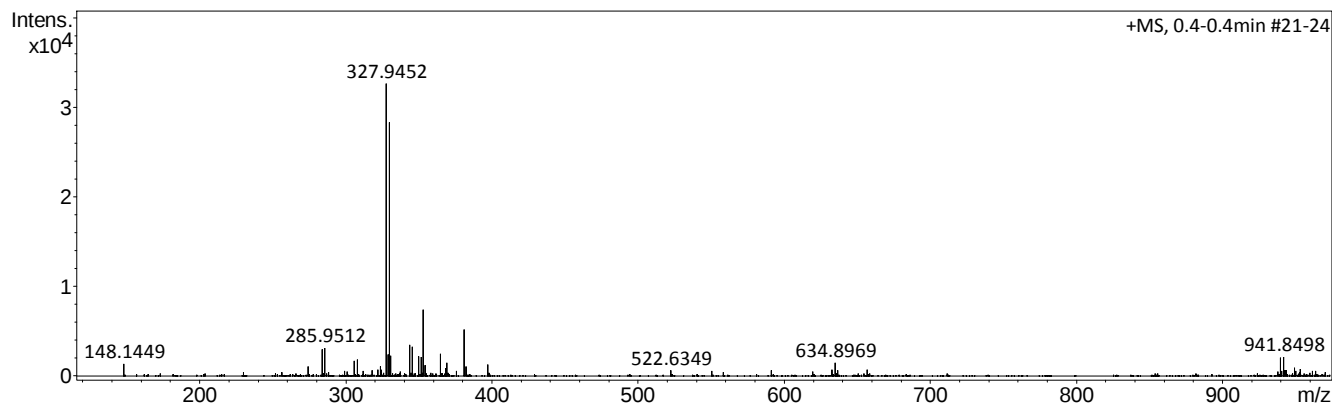

#	m/z	I	I %
1	148.1449	1356	4.2
2	274.2949	1069	3.3
3	283.9552	3008	9.2
4	285.9512	3124	9.6
5	305.9577	1758	5.4
6	307.9584	1870	5.7
7	323.9364	1070	3.3
8	327.9452	32588	100.0
9	328.9488	2405	7.4
10	329.9437	28275	86.8
11	330.5120	854	2.6
12	330.9482	2321	7.1
13	343.9248	3499	10.7
14	345.9221	3306	10.1
15	349.9288	2236	6.9
16	351.9257	2116	6.5
17	353.2946	7396	22.7
18	354.2956	1213	3.7
19	365.1369	2493	7.7
20	368.4495	846	2.6
21	369.2718	1487	4.6
22	381.3289	5182	15.9
23	382.3297	1101	3.4
24	397.3005	1332	4.1
25	632.8934	750	2.3
26	634.8969	1497	4.6
27	939.8364	2056	6.3
28	941.8498	2120	6.5
29	949.3661	959	2.9
30	953.3163	831	2.6