

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-120603_P1-B-7_01_9820.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-120603
 Comment SOL420
 Sv: DMSO + MeOH + HCOOH
 Mercedes Blanco

Acquisition Date 12/23/2024 12:30:33 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

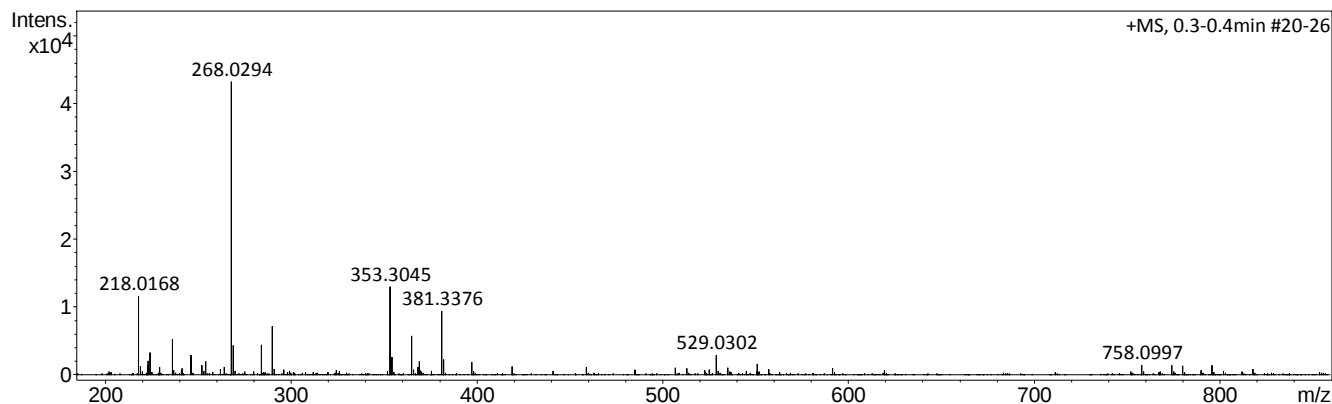

#	m/z	I	I %
1	218.0168	11629	26.9
2	219.0205	1222	2.8
3	222.6722	1367	3.2
4	223.0727	2073	4.8
5	224.0351	3362	7.8
6	236.0278	5299	12.3
7	246.0389	2905	6.7
8	252.0286	1432	3.3
9	254.0401	1977	4.6
10	264.0284	1195	2.8
11	268.0294	43187	100.0
12	269.0327	4326	10.0
13	284.0040	4411	10.2
14	290.0129	7156	16.6
15	353.3045	13013	30.1
16	354.3057	2623	6.1
17	365.1449	5763	13.3
18	368.4627	1133	2.6
19	369.2783	2003	4.6
20	381.3376	9460	21.9
21	382.3378	2303	5.3
22	397.3119	1906	4.4
23	419.0552	1285	3.0
24	459.0550	1170	2.7
25	529.0302	2897	6.7
26	551.0183	1603	3.7
27	758.0997	1473	3.4
28	774.0579	1409	3.3
29	780.0775	1380	3.2
30	796.0454	1399	3.2