

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-120604_P1-B-8_01_9821.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-120604
 Comment SOL443
 Sv: DMSO + MeOH + HCOOH
 Mercedes Blanco

Acquisition Date 12/23/2024 12:35:40 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

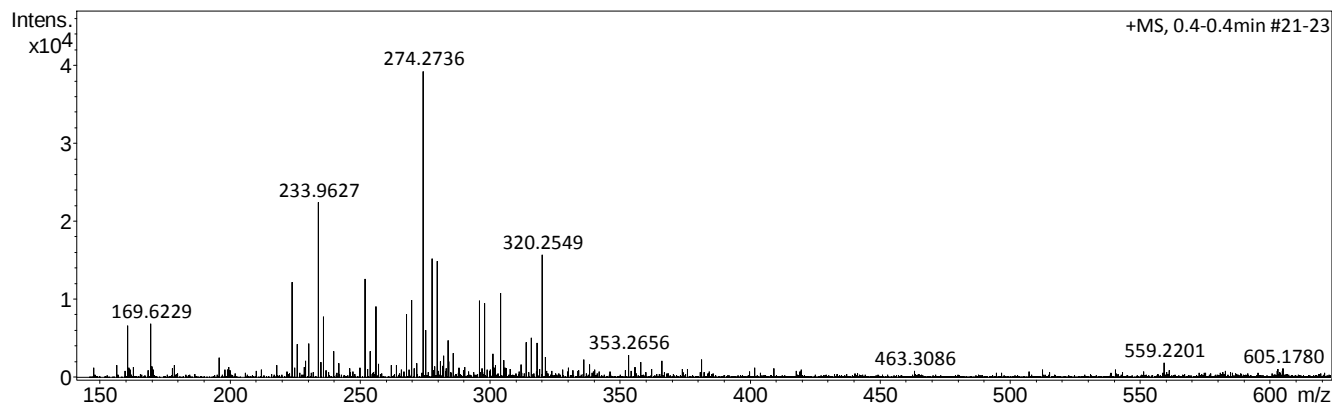

#	m/z	I	I %
1	160.6177	6621	16.9
2	169.6229	6843	17.5
3	224.0124	12145	31.0
4	226.0091	4282	10.9
5	230.2482	4350	11.1
6	233.9627	22404	57.2
7	235.9627	7759	19.8
8	239.9950	3316	8.5
9	251.9730	12544	32.1
10	253.9737	3358	8.6
11	256.2630	9056	23.1
12	267.9616	8111	20.7
13	269.9693	9887	25.3
14	274.2736	39137	100.0
15	275.2747	6023	15.4
16	277.9163	15234	38.9
17	279.9093	14874	38.0
18	282.2785	2811	7.2
19	283.9567	4714	12.0
20	285.9519	3128	8.0
21	295.9233	9836	25.1
22	297.9231	9449	24.1
23	301.2557	3023	7.7
24	304.2600	10762	27.5
25	313.9422	4506	11.5
26	315.9293	5047	12.9
27	318.2687	4423	11.3
28	320.2549	15689	40.1
29	321.2560	2613	6.7
30	353.2656	2869	7.3