

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\23-121301_P1-D-1_01_8616.d
 Method lc_ms_auto_pos_poen_150322.m
 Sample Name 23-121301
 Comment 5 min
 Carpinella

Acquisition Date 2/22/2024 12:27:39 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

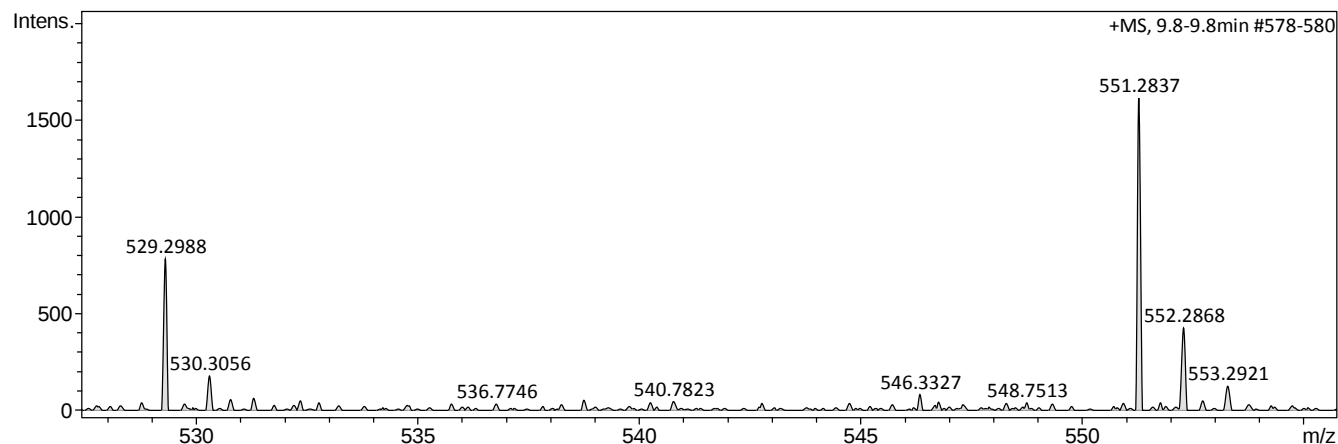

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
529.2988	1	C27H45O10	529.3007	3.6	38.1	2	34.47	5.5	even	ok
551.2837	1	C27H44NaO10	551.2827	-1.9	20.6	1	100.00	5.5	even	ok