

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\23-121302_P1-D-2_01_8617.d
 Method lc_ms_auto_pos_poen_150322.m
 Sample Name 23-121302
 Comment 6 min
 Carpinella

Acquisition Date 22/2/2024 2:06:53 p. m.

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

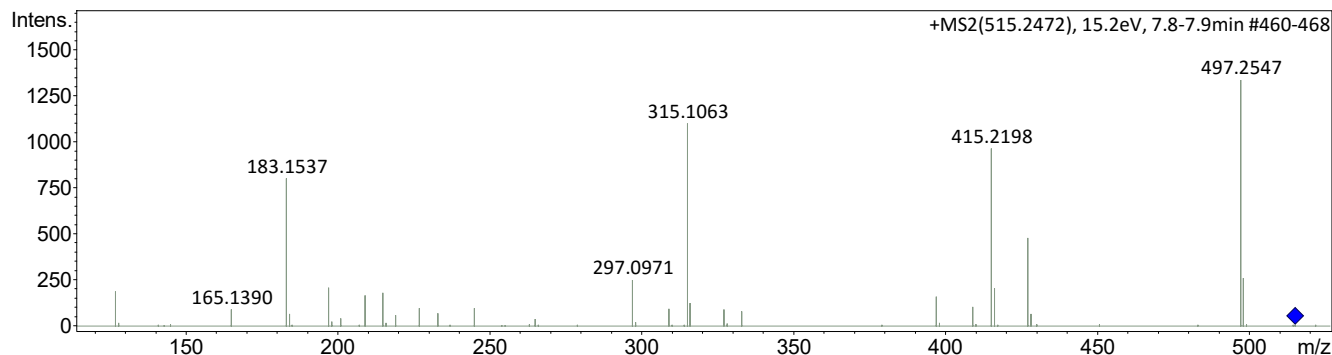

#	m/z	I	I %
1	127.0253	187	14.0
2	128.0300	19	1.4
3	165.1390	90	6.8
4	183.1537	801	60.1
5	184.1546	67	5.0
6	197.0586	209	15.7
7	198.0541	26	1.9
8	201.1604	42	3.1
9	209.0551	169	12.7
10	215.0637	183	13.7
11	219.1539	61	4.6
12	227.0637	98	7.3
13	233.0785	71	5.3
14	245.0724	97	7.3
15	265.0711	40	3.0
16	297.0971	252	18.9
17	298.1127	22	1.7
18	309.1718	95	7.1
19	315.1063	1100	82.5
20	316.1087	125	9.4
21	327.1808	92	6.9
22	333.1176	82	6.2
23	397.2102	161	12.1
24	409.2101	104	7.8
25	415.2198	964	72.3
26	416.2261	205	15.4
27	427.2215	478	35.9
28	428.2173	68	5.1
29	497.2547	1333	100.0
30	498.2558	261	19.6