

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\23-121304_P1-D-4_01_8619.d
Method lc_ms_auto_pos_poen_150322.m
Sample Name 23-121304
Comment 11 min
Carpinella

Acquisition Date 2/22/2024 2:48:59 PM

Operator ELB
Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

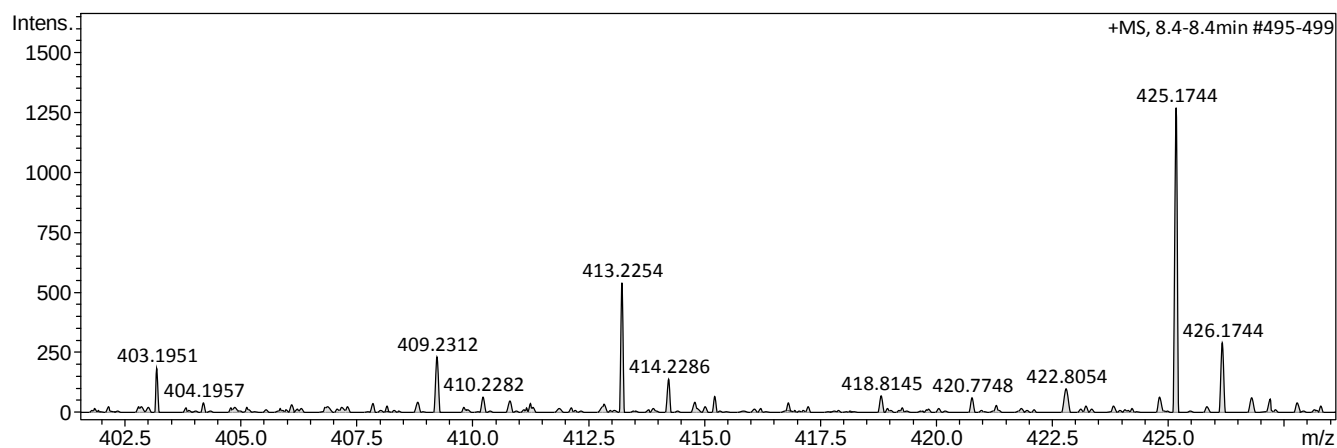

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
403.1951	1	C19H31O9	403.1963	2.8	23.9	1	100.00	4.5	even	ok
425.1744	1	C19H30NaO9	425.1782	8.9	25.0	1	9.08	4.5	even	ok