

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\EF50-N-VALERATO_P1-D-6_01_9679.d
 Method lc_ms directos tunelow300924.m
 Sample Name EF50-N-VALERATO
 Comment Sv: DCM + MeOH + HCOOH
 D'Accorso

Acquisition Date 11/11/2024 2:04:00 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

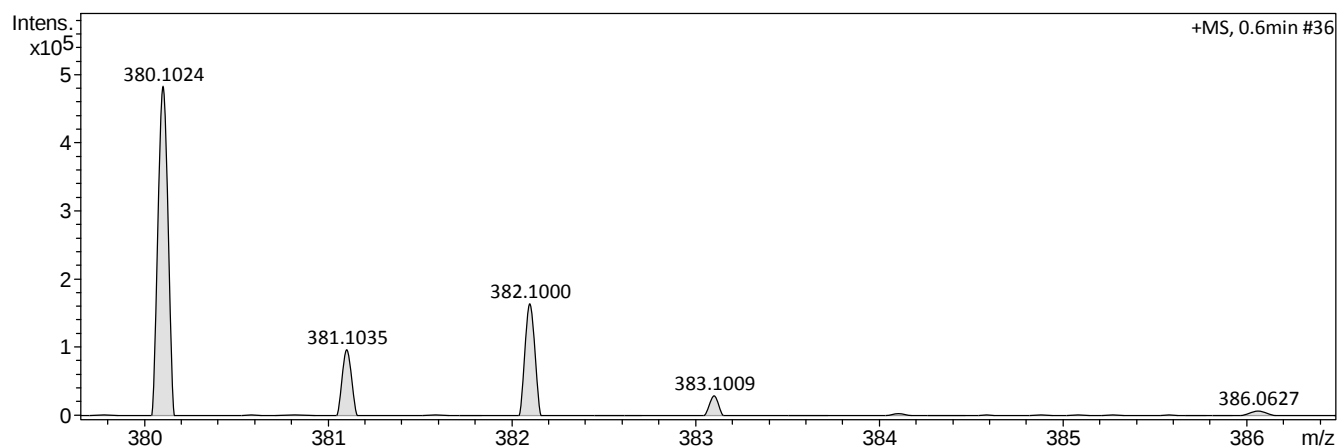

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
380.1024	1	C20H20CINNaO3	380.1024	-0.0	13.4	1	100.00	10.5	even	ok