

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\Let1_P1-C-2_01_8030.d
Method lc_qtof_directospos.m
Sample Name Let1
Comment Sv: MeOH + HCOOH
DAccorso

Acquisition Date 9/25/2023 4:00:05 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

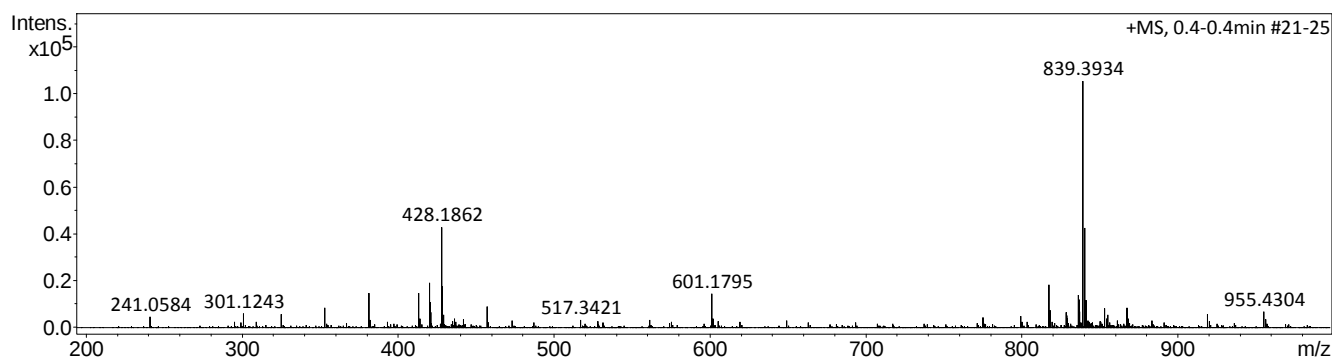

#	m/z	I	I %
1	241.0584	4698	4.5
2	301.1243	5994	5.7
3	325.2101	5671	5.4
4	353.2492	8371	8.0
5	381.2766	14794	14.1
6	413.2446	14766	14.1
7	420.1977	19094	18.2
8	420.6982	10857	10.3
9	421.2001	6547	6.2
10	428.1862	42749	40.7
11	428.6876	17387	16.5
12	429.1922	5499	5.2
13	457.2543	9006	8.6
14	601.1795	14455	13.8
15	799.4067	4941	4.7
16	817.4142	18309	17.4
17	818.4177	7284	6.9
18	828.4030	6471	6.2
19	828.9042	5185	4.9
20	836.3922	13916	13.2
21	836.8923	11910	11.3
22	837.3917	6864	6.5
23	839.3934	105068	100.0
24	840.3985	42618	40.6
25	841.4019	11735	11.2
26	853.4072	8167	7.8
27	855.3696	5493	5.2
28	867.4204	8378	8.0
29	919.4526	5684	5.4
30	955.4304	6910	6.6