

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\R10_P1-D-5_01_7912.d
 Method tune_high_pos hasta 2000.m
 Sample Name R10
 Comment Sv: Acetonitrilo + MeOH + HCOOH
 DAccorso

Acquisition Date 8/30/2023 1:08:39 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	1.0 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	400 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	2000 m/z	Set Collision Cell RF	800.0 Vpp	Set Divert Valve	Source

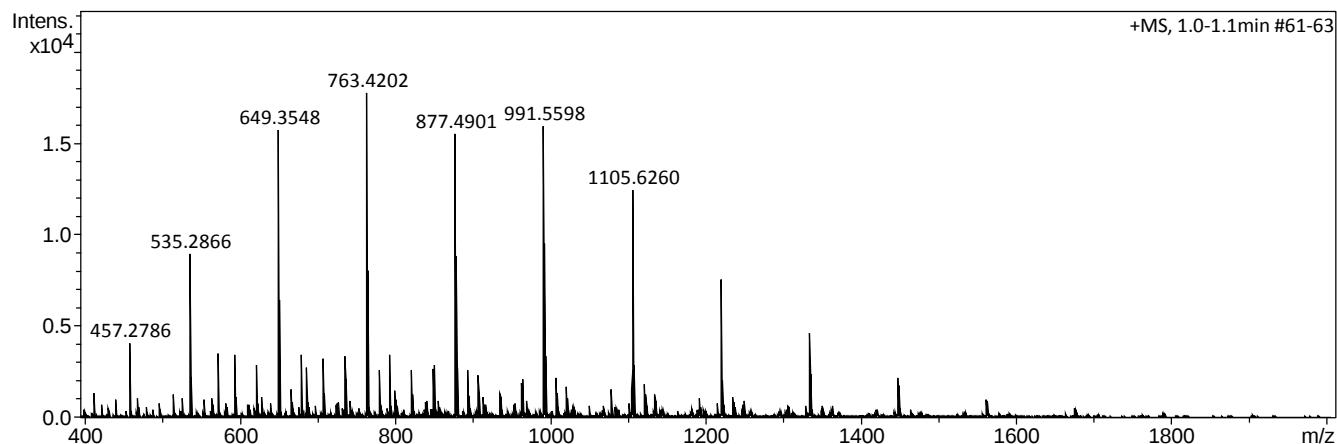

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
1105.6260	1	C57H94NaO19	1105.6282	2.0	30.9	1	100.00	10.5	even	ok
1219.6919	1	C63H104NaO21	1219.6962	3.6	37.3	1	100.00	11.5	even	ok
1333.7458	1	C69H114NaO23	1333.7643	13.9	39.6	1	0.52	12.5	even	ok
1447.8293	1	C75H124NaO25	1447.8324	2.1	67.2	1	100.00	13.5	even	ok
1561.8979	1	C81H134NaO27	1561.9005	1.6	414.0	1	100.00	14.5	even	ok
1675.9437	1	C87H144NaO29	1675.9685	14.8	47.8	2	0.00	15.5	even	ok