

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\R7_P1-D-2_01_7896.d
 Method lc_qtof_directospos.m
 Sample Name R7
 Comment Sv: Acetonitrilo + MeOH + HCOOH
 DAccorso

Acquisition Date 8/28/2023 12:52:04 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

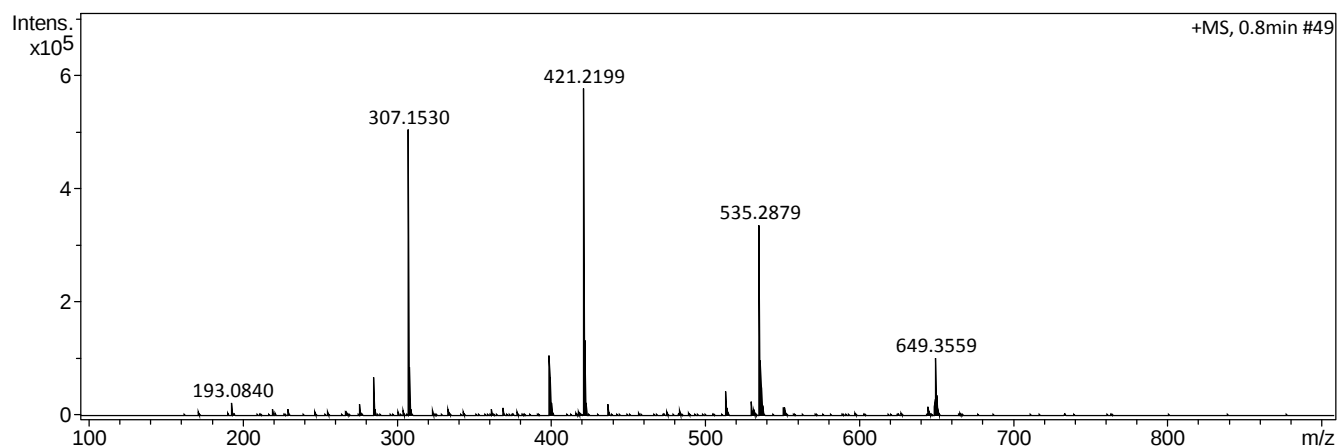

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
285.1702	1	C15H25O5	285.1697	-2.0	9.2	1	100.00	3.5	even	ok
307.1530	1	C15H24NaO5	307.1516	-4.5	1.0	1	60.74	3.5	even	ok
399.2377	1	C21H35O7	399.2377	0.1	8.4	1	100.00	4.5	even	ok
421.2199	1	C21H34NaO7	421.2197	-0.5	3.1	1	100.00	4.5	even	ok
513.3043	1	C27H45O9	513.3058	2.9	11.1	1	100.00	5.5	even	ok
535.2879	1	C27H44NaO9	535.2878	-0.3	7.5	1	100.00	5.5	even	ok
649.3559	1	C33H54NaO11	649.3558	-0.1	7.9	1	100.00	6.5	even	ok