

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\MTA39_P1-D-8_01_9183.d
 Method lc_qtof_directospos.m
 Sample Name MTA39
 Comment Sv: DMSO + MeOH + HCOOH
 Di Chenna

Acquisition Date 5/16/2024 11:47:06 AM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

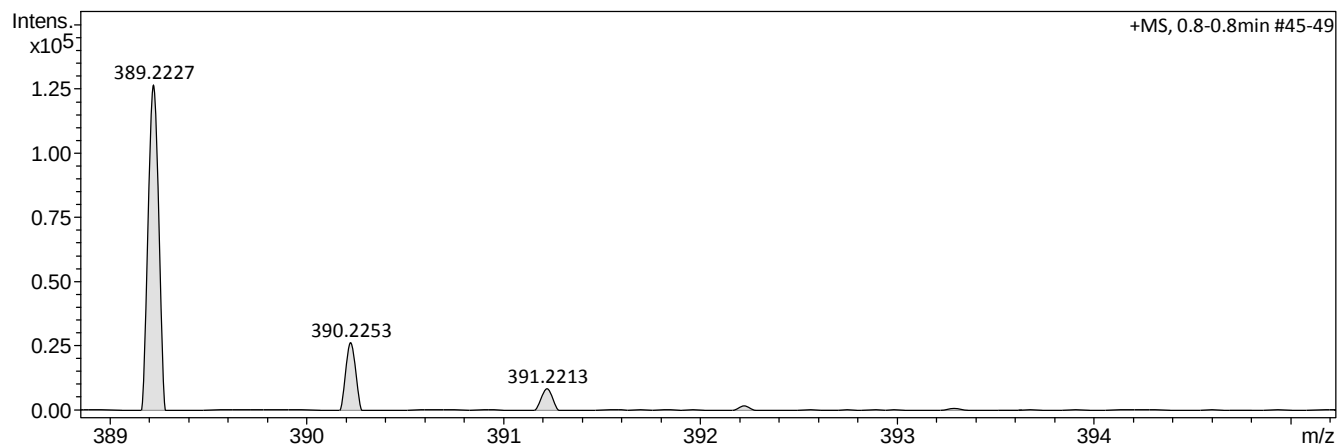

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
389.2227	1	C17H33N4O4S	389.2217	-2.5	4.5	1	100.00	3.5	even	ok