

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\V100F10p255_P1-E-3_01_9719.d
 Method lc-qtof directos tune high 141124 pos.m
 Sample Name V100F10p255
 Comment Sv: MeOH + Agua
 Di Chenna

Acquisition Date 11/14/2024 3:13:22 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3000 V	Set Dry Heater	200 °C
Scan Begin	400 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	3100 m/z	Set Collision Cell RF	700.0 Vpp	Set Divert Valve	Source

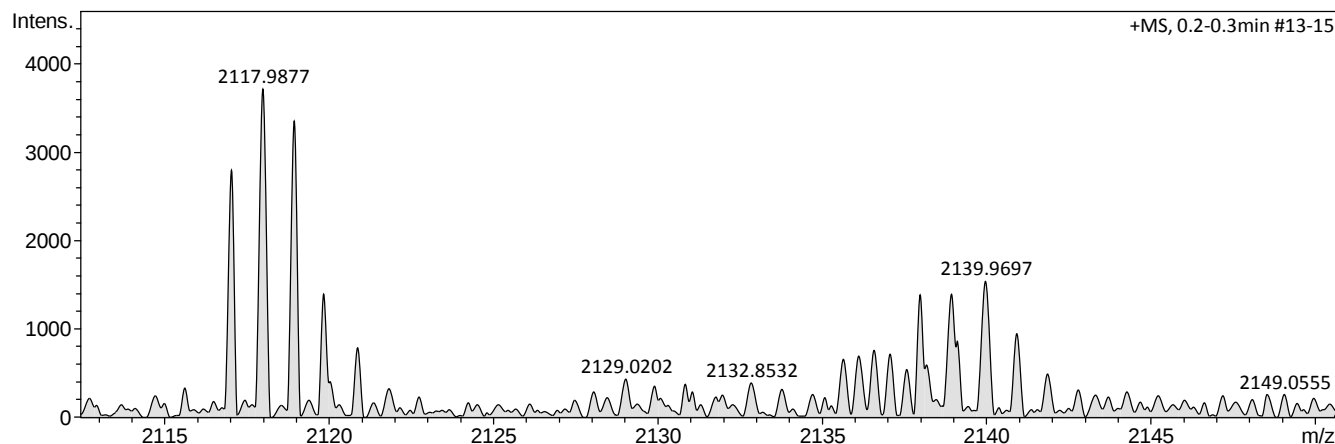

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
2117.9877	1	C92H153N18O30S4	2117.9877	0.0	317.1	1	100.00	25.5	even	ok
2139.9697	1	C92H152N18NaO30S4	2139.9697	0.0	374.1	1	100.00	25.5	even	ok