

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\V77p191_P1-F-7_01_8754.d
 Method lc_qtof_directospos.m
 Sample Name V77p191
 Comment Sv: MeOH + HCOOH
 Di Chenna

Acquisition Date 3/18/2024 6:17:06 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

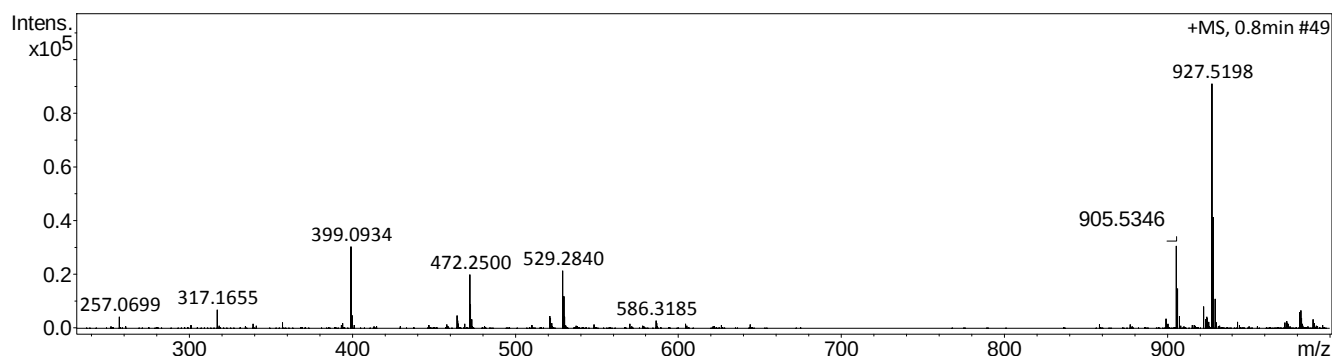

#	m/z	I	I %
1	257.0699	4258	4.7
2	317.1655	6880	7.6
3	399.0934	30432	33.4
4	400.0999	4783	5.3
5	464.2606	4824	5.3
6	464.7644	2859	3.1
7	472.2500	19890	21.9
8	472.7512	8775	9.6
9	473.2546	3335	3.7
10	521.2960	4674	5.1
11	521.7946	3761	4.1
12	529.2840	21502	23.6
13	529.7852	11817	13.0
14	530.2890	4249	4.7
15	586.3185	2869	3.2
16	899.4879	3517	3.9
17	905.5346	30625	33.6
18	906.5356	14701	16.2
19	907.5382	4481	4.9
20	922.5640	8161	9.0
21	923.5634	3437	3.8
22	924.5177	4299	4.7
23	925.0157	3566	3.9
24	927.5198	91027	100.0
25	928.5225	41269	45.3
26	929.5242	11065	12.2
27	981.5487	5941	6.5
28	982.0495	6681	7.3
29	982.5447	3792	4.2
30	989.4986	3488	3.8