

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\V77p191_P1-F-7_01_8754.d
 Method lc_qtof_directospos.m
 Sample Name V77p191
 Comment Sv: MeOH + HCOOH
 Di Chenna

Acquisition Date 3/18/2024 6:17:06 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

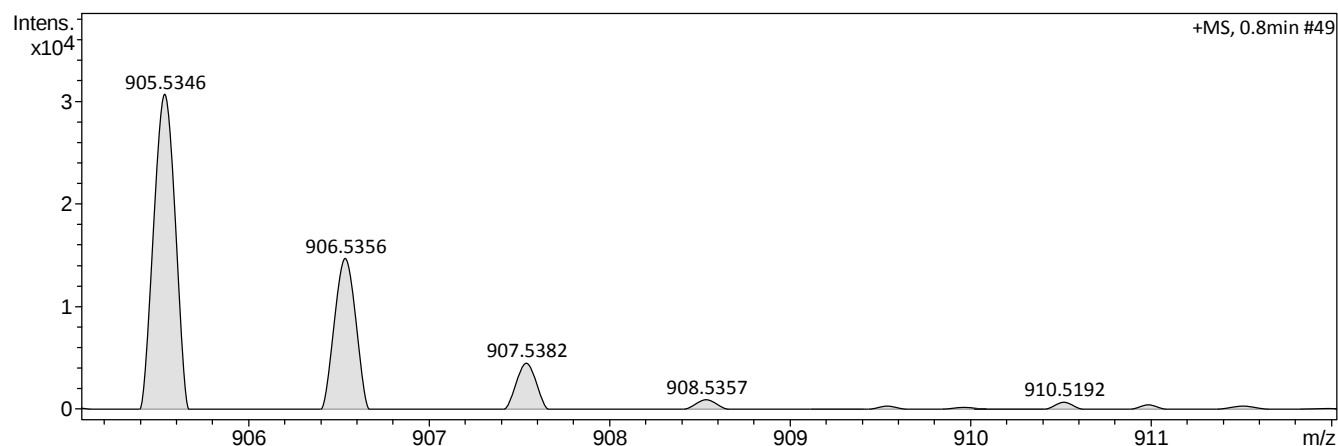

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
905.5346	1	C40H69N14O10	905.5316	-3.3	8.3	1	47.11	13.5	even	ok