

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\V82p200_P1-F-6_01_8753.d
 Method lc_qtof_directospos.m
 Sample Name V82p200
 Comment Sv: MeOH + HCOOH
 Di Chenna

Acquisition Date 3/18/2024 6:11:59 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

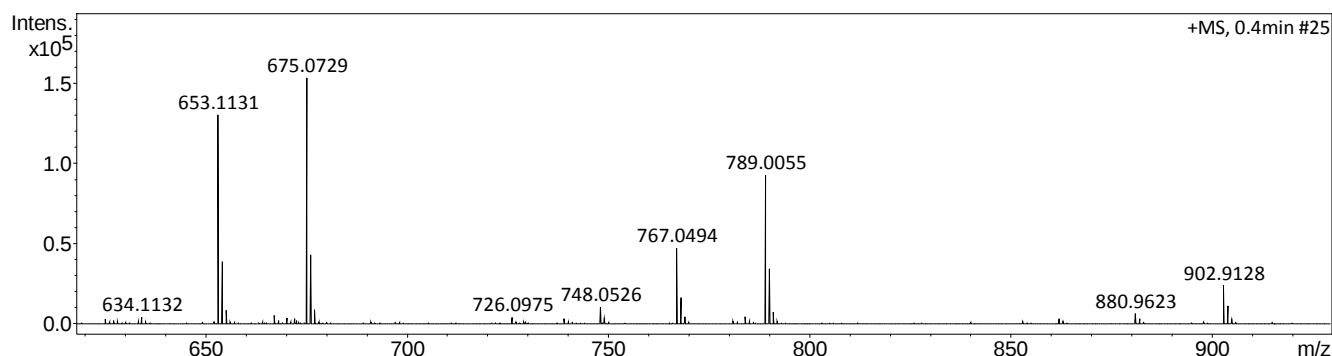

#	m/z	I	I %
1	473.2796	2415	1.6
2	495.1257	2670	1.7
3	625.1341	2746	1.8
4	634.1132	4045	2.6
5	653.1131	129832	84.9
6	654.1124	38789	25.4
7	655.1108	8359	5.5
8	667.0975	5408	3.5
9	670.1217	3794	2.5
10	672.0748	3469	2.3
11	675.0729	152841	100.0
12	676.0724	43010	28.1
13	677.0710	9027	5.9
14	726.0975	4171	2.7
15	739.0699	3316	2.2
16	748.0526	10331	6.8
17	749.0580	3707	2.4
18	767.0494	46941	30.7
19	768.0536	16560	10.8
20	769.0517	4364	2.9
21	784.0571	4340	2.8
22	789.0055	92687	60.6
23	790.0043	34458	22.5
24	791.0035	7241	4.7
25	861.9729	3389	2.2
26	880.9623	6495	4.2
27	881.9629	3308	2.2
28	902.9128	24027	15.7
29	903.9083	11103	7.3
30	904.9162	2796	1.8