

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\V86p206_P1-B-9_01_9664.d
 Method tunelow300924 50 a 1500.m
 Sample Name V86p206
 Comment Sv: DCM + MeOH + HCOOH
 Di Chenna


Acquisition Date 11/8/2024 1:28:17 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

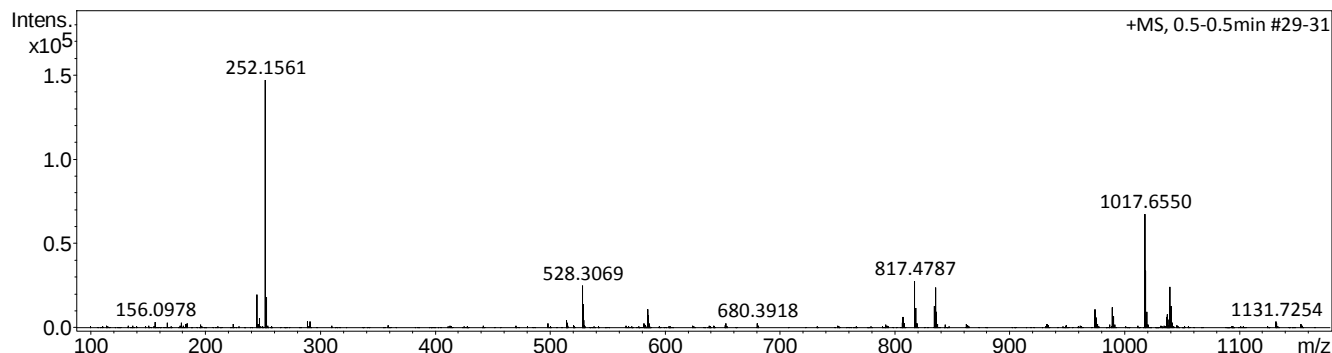

#	m/z	I	I %
1	245.1158	19661	13.4
2	247.1143	5840	4.0
3	252.1561	146841	100.0
4	253.1567	18276	12.4
5	289.0650	3935	2.7
6	291.0617	3904	2.7
7	514.2990	4599	3.1
8	528.3069	25175	17.1
9	528.8068	13911	9.5
10	529.3096	4453	3.0
11	585.3416	11081	7.5
12	585.8446	7207	4.9
13	807.4861	6586	4.5
14	817.4787	27629	18.8
15	818.4776	11709	8.0
16	834.5619	12900	8.8
17	835.5066	23931	16.3
18	836.5064	9548	6.5
19	974.6317	11054	7.5
20	975.6297	6261	4.3
21	989.6349	11983	8.2
22	990.6493	6803	4.6
23	1017.6550	67510	46.0
24	1018.6577	33902	23.1
25	1019.6470	9357	6.4
26	1036.6349	6352	4.3
27	1037.1354	8123	5.5
28	1037.6327	5031	3.4
29	1039.6260	24388	16.6
30	1040.6376	13004	8.9