

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\V86p206_P1-B-9_01_9664.d
 Method tunelow300924 50 a 1500.m
 Sample Name V86p206
 Comment Sv: DCM + MeOH + HCOOH
 Di Chenna

Acquisition Date 11/8/2024 1:28:17 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

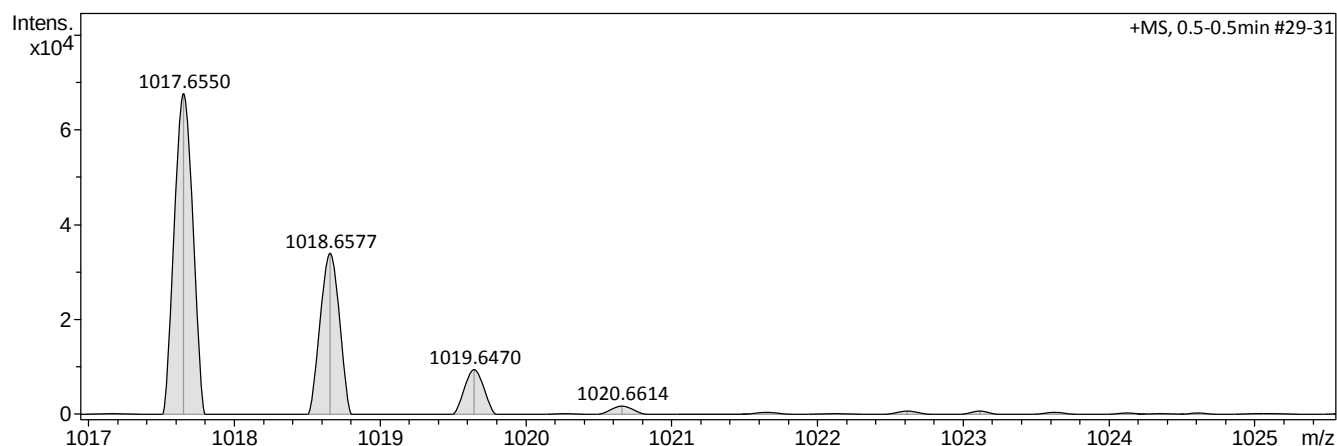

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
1017.6550	1	C48H85N14O10	1017.6568	1.8	92.1	1	100.00	13.5	even	ok