

# Mass Spectrum List Report

## Analysis Info


Analysis Name D:\Data\ggc\24-112702.d  
 Method tunelow300924.m  
 Sample Name SN4-C7  
 Comment Sv: CDM + MeOH + HCOOH  
 Florencia Di Salvo

Acquisition Date 12/3/2024 12:14:38 PM

Operator EB - MV  
 Instrument / Ser# microTOF-Q

## Acquisition Parameter

|             |            |                       |           |                  |           |
|-------------|------------|-----------------------|-----------|------------------|-----------|
| Source Type | ESI        | Ion Polarity          | Positive  | Set Nebulizer    | 0.4 Bar   |
| Focus       | Not active | Set Capillary         | 4000 V    | Set Dry Heater   | 200 °C    |
| Scan Begin  | 50 m/z     | Set End Plate Offset  | -500 V    | Set Dry Gas      | 4.0 l/min |
| Scan End    | 1000 m/z   | Set Collision Cell RF | 200.0 Vpp | Set Divert Valve | Source    |

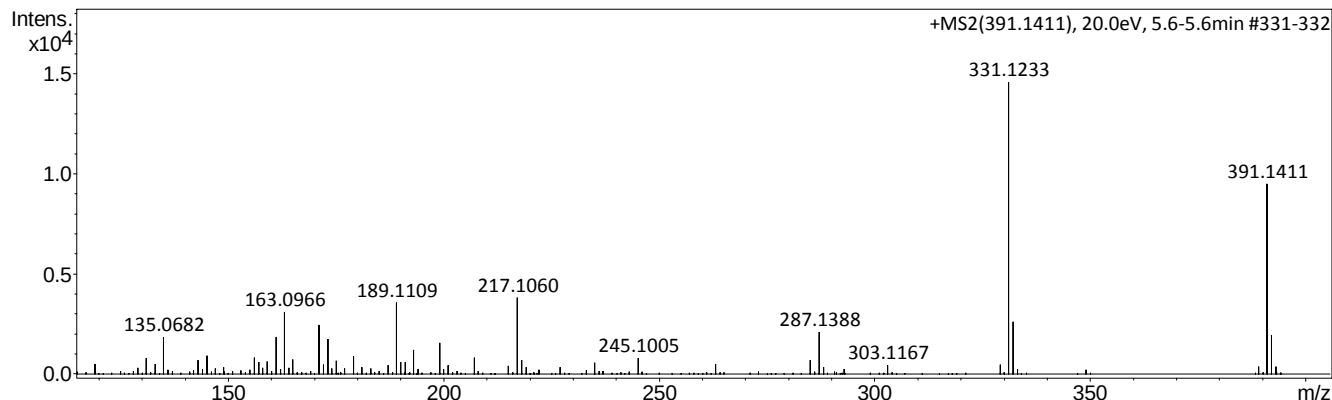

| #  | m/z      | I     | I %   |
|----|----------|-------|-------|
| 1  | 131.0738 | 817   | 5.6   |
| 2  | 135.0682 | 1863  | 12.8  |
| 3  | 143.0726 | 717   | 4.9   |
| 4  | 145.0854 | 919   | 6.3   |
| 5  | 156.0810 | 847   | 5.8   |
| 6  | 157.0875 | 619   | 4.3   |
| 7  | 159.0951 | 637   | 4.4   |
| 8  | 161.1158 | 1842  | 12.7  |
| 9  | 163.0966 | 3080  | 21.2  |
| 10 | 165.0108 | 726   | 5.0   |
| 11 | 171.1017 | 2471  | 17.0  |
| 12 | 173.1147 | 1761  | 12.1  |
| 13 | 175.0912 | 686   | 4.7   |
| 14 | 179.0569 | 889   | 6.1   |
| 15 | 189.1109 | 3568  | 24.5  |
| 16 | 190.1139 | 621   | 4.3   |
| 17 | 191.1256 | 605   | 4.2   |
| 18 | 193.0325 | 1232  | 8.5   |
| 19 | 199.0946 | 1579  | 10.8  |
| 20 | 207.0892 | 834   | 5.7   |
| 21 | 217.1060 | 3817  | 26.2  |
| 22 | 218.1070 | 708   | 4.9   |
| 23 | 235.1143 | 579   | 4.0   |
| 24 | 245.1005 | 809   | 5.6   |
| 25 | 285.1007 | 711   | 4.9   |
| 26 | 287.1388 | 2096  | 14.4  |
| 27 | 331.1233 | 14557 | 100.0 |
| 28 | 332.1260 | 2616  | 18.0  |
| 29 | 391.1411 | 9476  | 65.1  |
| 30 | 392.1423 | 1962  | 13.5  |