

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\LR-MM-5_P1-C-1_01_8333.d
Method lc_qtof_directospos.m
Sample Name LR-MM-5
Comment Sv: DCM + MeOH + HCOOH
Durán

Acquisition Date 12/6/2023 10:04:24 AM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

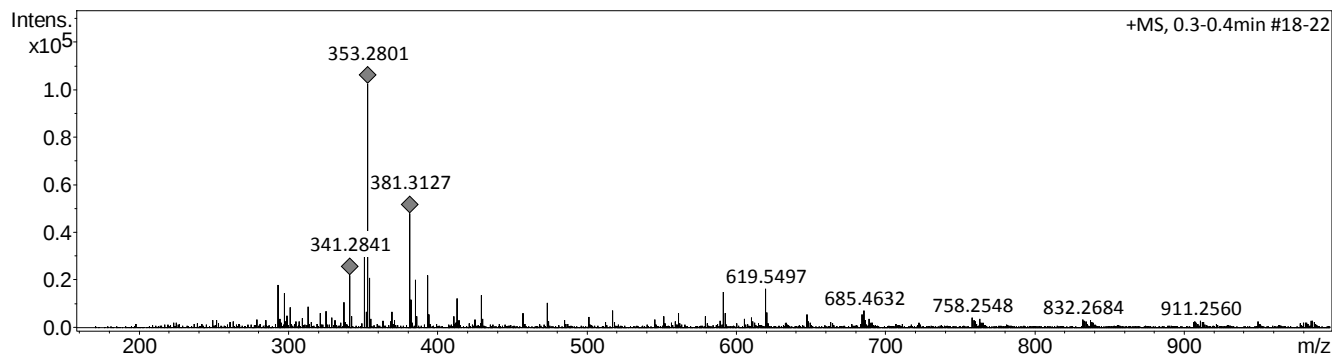

#	m/z	I	I %
1	293.2196	17976	17.6
2	297.2494	14480	14.2
3	301.1468	8498	8.3
4	313.2818	8720	8.5
5	321.2493	6117	6.0
6	325.2586	6904	6.8
7	337.2458	10629	10.4
8	341.2841	21929	21.4
9	351.1706	31664	31.0
10	352.1751	6550	6.4
11	353.2801	102241	100.0
12	354.2837	20798	20.3
13	369.3107	6668	6.5
14	381.3127	47987	46.9
15	382.3150	11692	11.4
16	385.3060	20080	19.6
17	393.3132	21908	21.4
18	413.3002	12334	12.1
19	429.3345	13736	13.4
20	457.3629	6190	6.1
21	473.3625	10464	10.2
22	517.3911	7264	7.1
23	561.4177	6008	5.9
24	591.5191	14943	14.6
25	592.5251	6072	5.9
26	619.5497	16282	15.9
27	620.5541	6299	6.2
28	647.5898	5542	5.4
29	684.2342	5469	5.3
30	685.4632	7061	6.9