

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\LR-MM-5_P1-C-1_01_8335.d
Method appi lcms 200.m
Sample Name LR-MM-5
Comment Sv: DCM + MeOH + HCOOH
Durán

Acquisition Date 12/6/2023 11:45:20 AM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	APPI	Ion Polarity	Positive	Set Nebulizer	3.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	100 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	6.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

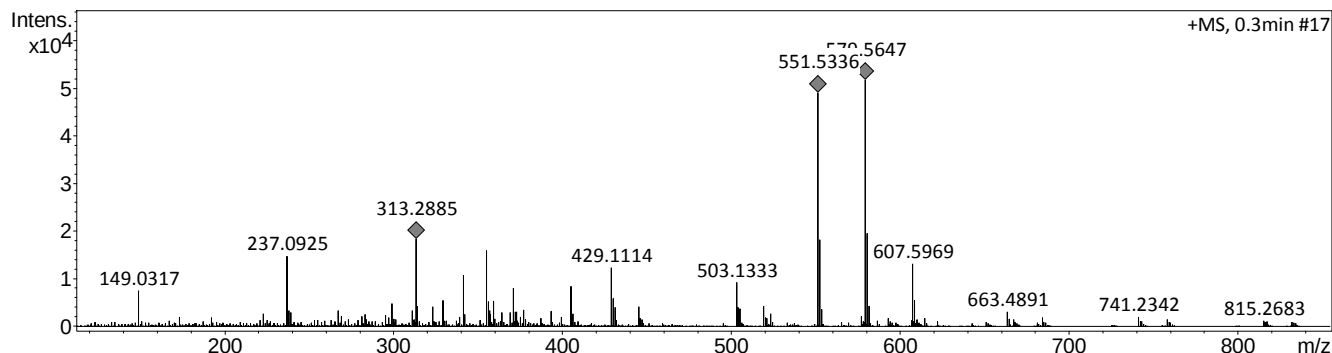

#	m/z	I	I %
1	149.0317	7504	14.5
2	237.0925	14707	28.5
3	299.0785	4794	9.3
4	313.2885	18325	35.5
5	314.2914	4303	8.3
6	323.2180	4142	8.0
7	329.1959	5446	10.5
8	341.3184	10678	20.7
9	355.0884	15978	30.9
10	356.0901	5175	10.0
11	359.2384	5421	10.5
12	371.1183	7986	15.5
13	377.2480	3460	6.7
14	405.2469	8424	16.3
15	429.1114	12323	23.9
16	430.1097	5865	11.4
17	431.1099	3986	7.7
18	445.1413	4140	8.0
19	503.1333	9252	17.9
20	504.1321	4080	7.9
21	505.1335	3745	7.3
22	519.1657	4231	8.2
23	551.5336	48935	94.7
24	552.5341	18213	35.3
25	553.5351	3554	6.9
26	579.5647	51651	100.0
27	580.5679	19570	37.9
28	581.5699	4304	8.3
29	607.5969	13087	25.3
30	608.5992	5491	10.6