

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\LR-MM-7_P1-C-7_01_8265.d
Method lc_qtof_directospos.m
Sample Name LR-MM-7
Comment Sv: MeOH + HCOOH
Durán

Acquisition Date 11/2/2023 2:22:51 PM

Operator ELB
Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

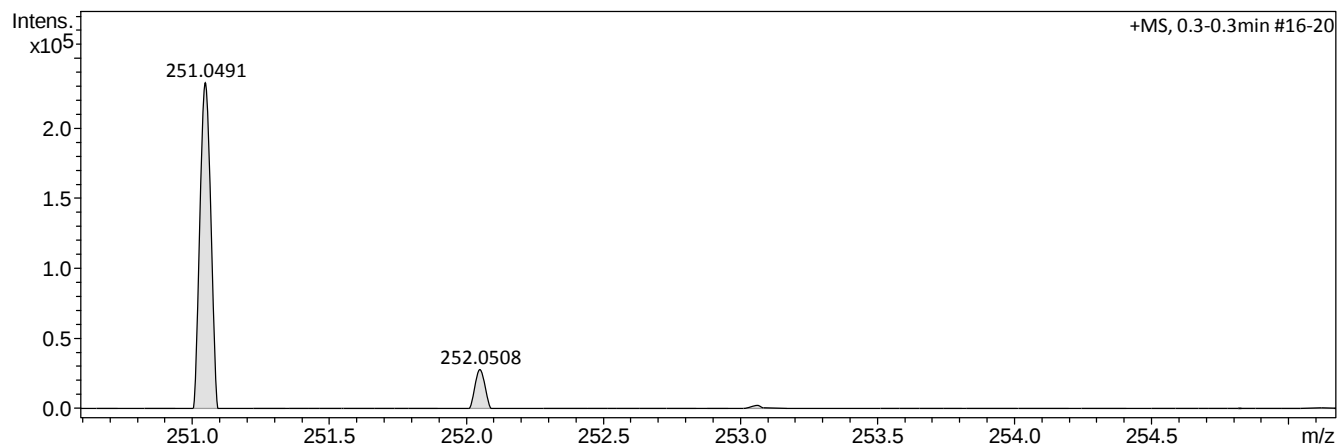

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	#	mSigma	Score	rdb	e ⁻ Conf	N-Rule
251.0491	1	C ₁₁ H ₁₀ F ₂ NaO ₃	251.0490	-0.2	1.4	1	1	100.00	5.5	even	ok