

# Qualitative Compound Report

## Analysis Info

Analysis Name D:\Data\ggc\LR1-122\_P1-D-5\_01\_7534.d  
Method lc\_qtof\_directospos.m  
Sample Name LR1-122  
Comment Sv: DCM + MeOH + HCOOH  
Duran


Acquisition Date 7/14/2023 3:30:26 PM

Operator ELB  
Instrument micrOTOF-Q II



## Acquisition Parameter

|             |            |                       |           |                  |           |
|-------------|------------|-----------------------|-----------|------------------|-----------|
| Source Type | ESI        | Ion Polarity          | Positive  | Set Nebulizer    | 3.5 Bar   |
| Focus       | Not active | Set Capillary         | 4000 V    | Set Dry Heater   | 200 °C    |
| Scan Begin  | 70 m/z     | Set End Plate Offset  | -500 V    | Set Dry Gas      | 7.0 l/min |
| Scan End    | 1000 m/z   | Set Collision Cell RF | 300.0 Vpp | Set Divert Valve | Source    |

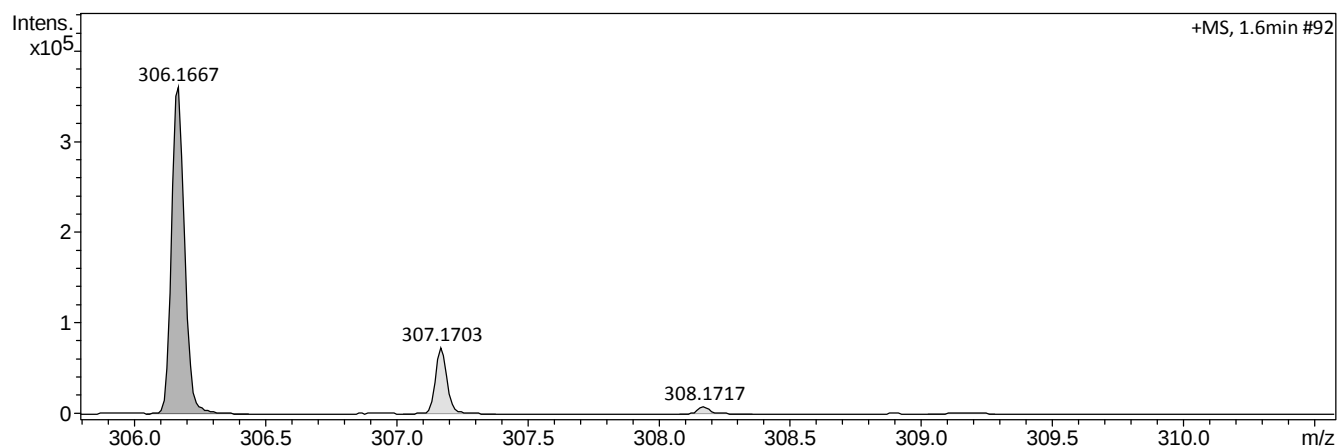

| Meas. m/z | # | Ion Formula | m/z      | err [ppm] | mSigma | # mSigma | Score  | rdb | e <sup>-</sup> Conf | N-Rule |
|-----------|---|-------------|----------|-----------|--------|----------|--------|-----|---------------------|--------|
| 306.1667  | 1 | C18H22F2NO  | 306.1664 | -1.0      | 1.0    | 1        | 100.00 | 7.5 | even                | ok     |