

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\LR1-123_P1-D-6_01_7535.d
Method lc_qtof_directospos.m
Sample Name LR1-123
Comment Sv: DCM + MeOH + HCOOH
Duran


Acquisition Date 7/14/2023 3:35:32 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

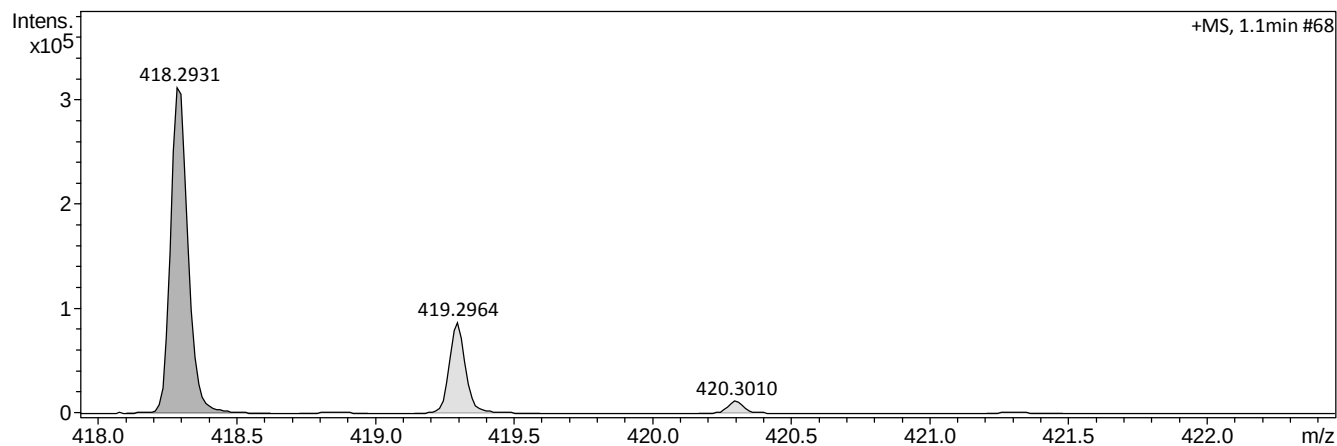

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
418.2931	1	C ₂₆ H ₃₈ F ₂ NO	418.2916	-3.5	7.5	2	56.03	7.5	even	ok