

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\LR1-146_P1-E-6_01_9686.d
 Method lc_ms directos tunelow300924.m
 Sample Name LR1-146
 Comment Sv: MeOH + HCOOH
 Fernando Durán


Acquisition Date 11/11/2024 3:26:50 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

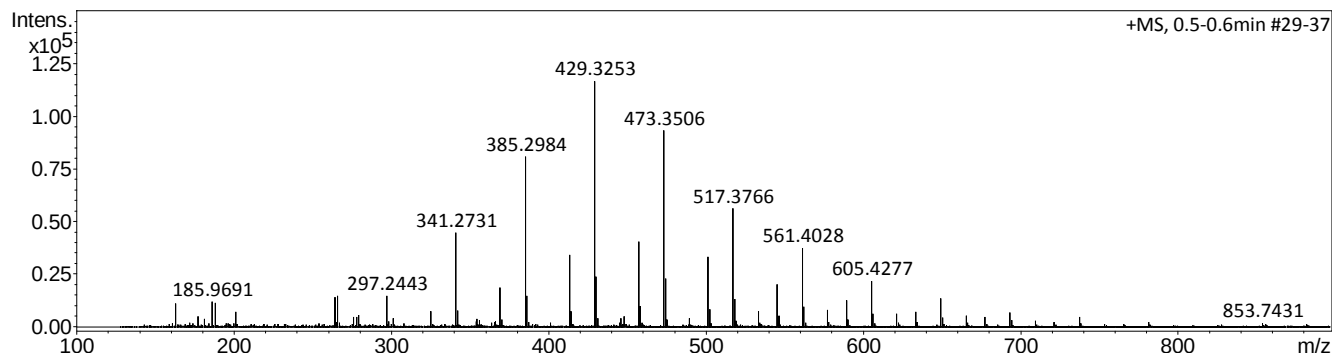

#	m/z	I	I %
1	163.0891	11172	9.6
2	185.9691	12001	10.3
3	187.9684	11361	9.8
4	264.0193	13959	12.0
5	266.0176	14588	12.5
6	297.2443	14694	12.6
7	341.2731	44535	38.3
8	342.2736	7681	6.6
9	369.3017	18702	16.1
10	385.2984	80784	69.4
11	386.2997	14832	12.7
12	413.3259	34128	29.3
13	414.3317	7565	6.5
14	429.3253	116397	100.0
15	430.3282	23907	20.5
16	457.3554	40406	34.7
17	458.3598	9967	8.6
18	473.3506	93014	79.9
19	474.3534	22769	19.6
20	501.3796	33240	28.6
21	502.3864	8461	7.3
22	517.3766	56305	48.4
23	518.3800	13348	11.5
24	545.4100	20237	17.4
25	561.4028	37395	32.1
26	562.4051	9629	8.3
27	577.3783	8013	6.9
28	589.4335	12534	10.8
29	605.4277	21556	18.5
30	649.4525	13385	11.5