

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\LR1-44_P1-D-1_01_4505.d
Method lc_qtof_directospos.m
Sample Name LR1-44
Comment Sv: DCM + MeOH
Mauricio Lisandro Ronconi / Lab. Durán


Acquisition Date 4/6/2022 10:57:41 AM

Operator GC
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

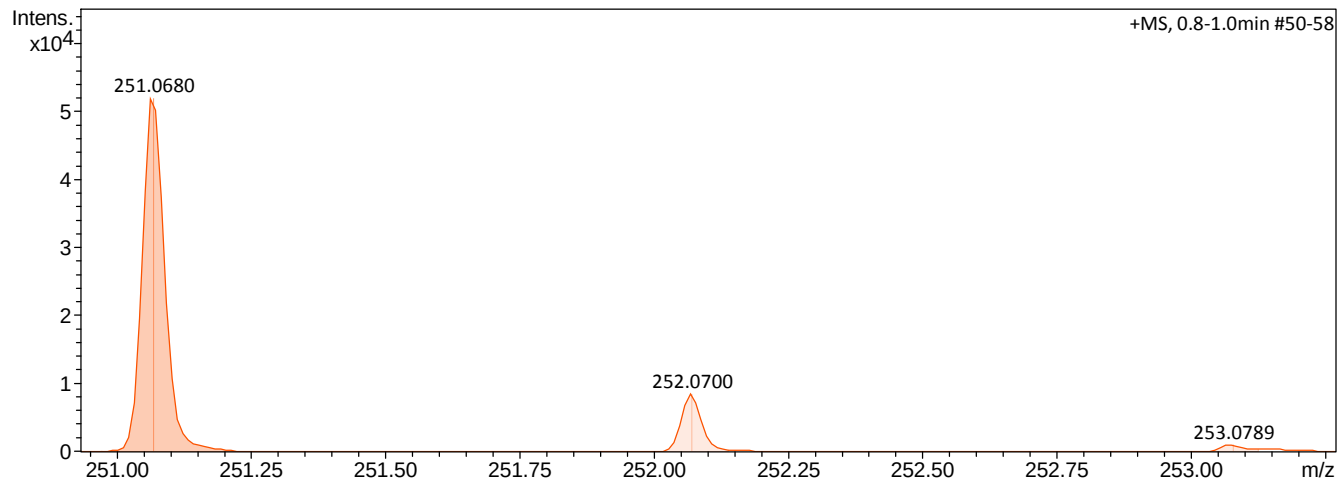

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
251.0680	1	C14H12NaO3	251.0679	-0.7	5.5	1	100.00	8.5	even	ok