

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\LR1-49_P1-D-2_01_4506.d
Method lc_qtof_directospos.m
Sample Name LR1-49
Comment Sv: DCM + MeOH
Mauricio Lisandro Ronconi / Lab. Durán


Acquisition Date 4/6/2022 11:02:52 AM

Operator GC
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

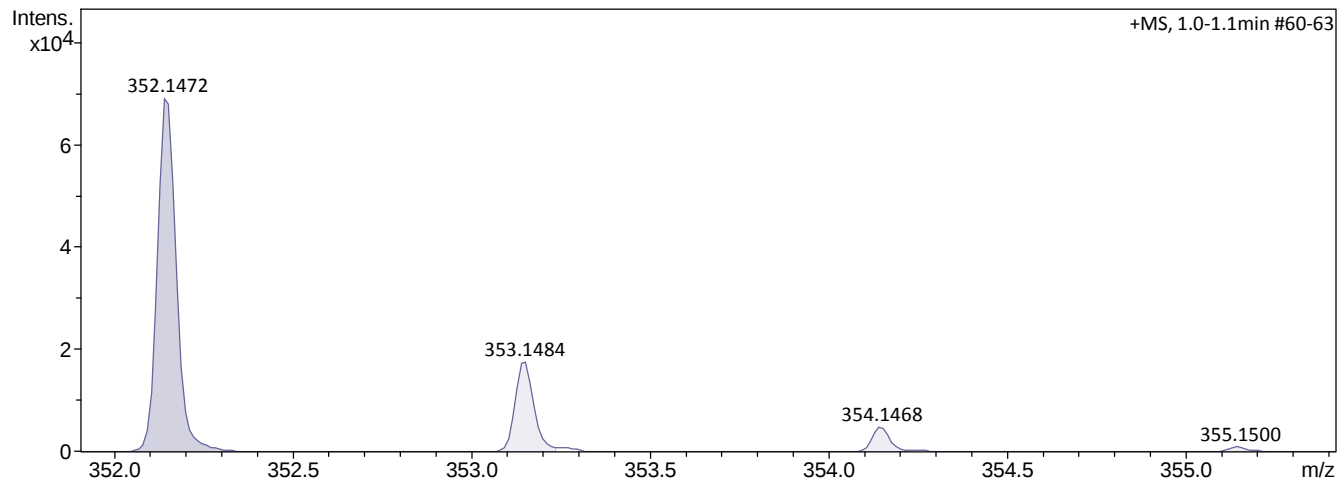

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
352.1472	1	C19H22N3O2Si	352.1476	1.2	9.3	1	100.00	11.5	even	ok