

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\LR1-55_P1-D-3_01_6203.d
Method lc_qtof_directospos.m
Sample Name LR1-55
Comment Sv: DCM + MeOH + HCOOH
Durán

Acquisition Date 12/15/2022 3:45:38 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

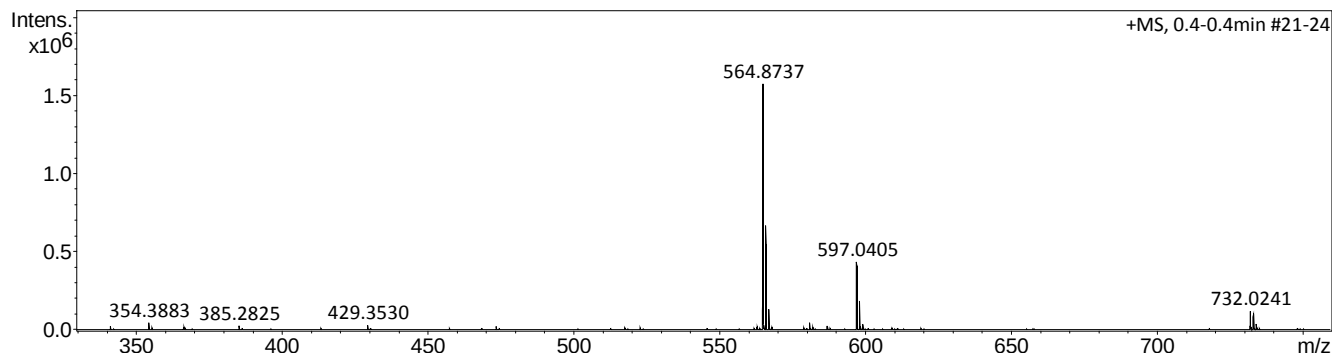

#	m/z	I	I %
1	341.2429	21953	1.4
2	354.3883	45115	2.9
3	355.3903	11617	0.7
4	366.3286	17201	1.1
5	366.8299	9809	0.6
6	385.2825	27279	1.7
7	413.3374	8729	0.6
8	429.3530	28460	1.8
9	457.4290	8893	0.6
10	473.4582	19930	1.3
11	517.5970	11982	0.8
12	522.8403	14575	0.9
13	562.8451	18453	1.2
14	564.8737	1573040	100.0
15	565.8809	664395	42.2
16	566.8866	131878	8.4
17	567.8939	14722	0.9
18	578.9111	13769	0.9
19	580.9352	45694	2.9
20	581.9436	18353	1.2
21	586.9478	22021	1.4
22	587.9574	8992	0.6
23	597.0405	433265	27.5
24	598.0491	185266	11.8
25	599.0569	38117	2.4
26	619.1285	8483	0.5
27	732.0241	121342	7.7
28	733.0440	102551	6.5
29	734.0618	36302	2.3
30	1156.5583	9014	0.6