

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\LR1-78-f24-39_P1-C-6_01_6197.d
Method lc_qtof_directospos.m
Sample Name LR1-78-f24-39
Comment Sv: DCM + MeOH + HCOOH
Durán

Acquisition Date 12/15/2022 3:14:58 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

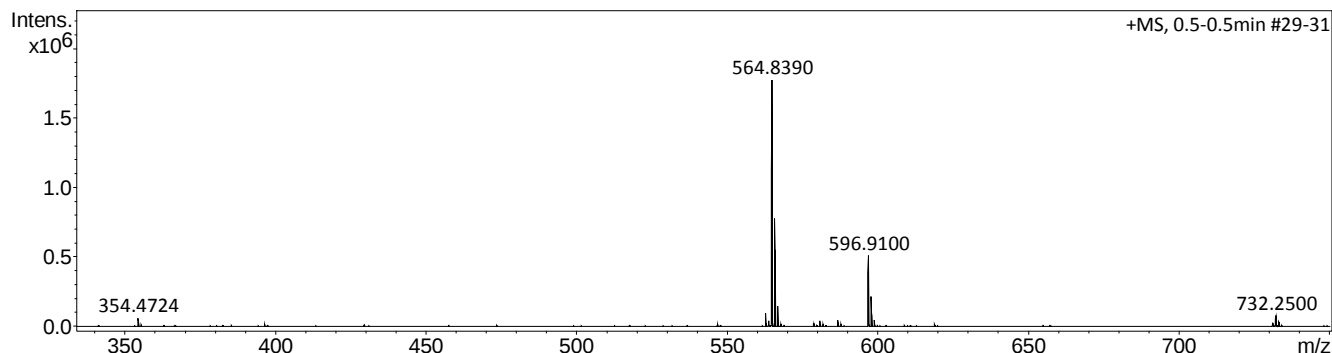

#	m/z	I	I %
1	354.4724	59245	3.3
2	355.4763	14474	0.8
3	396.4067	19695	1.1
4	429.4804	9670	0.5
5	546.7999	16486	0.9
6	562.8192	98810	5.6
7	563.8247	40912	2.3
8	564.8390	1769729	100.0
9	565.8433	775758	43.8
10	566.8474	147822	8.4
11	567.8521	16660	0.9
12	578.8410	18674	1.1
13	580.8563	41087	2.3
14	581.8597	17433	1.0
15	586.8511	48286	2.7
16	587.8561	19143	1.1
17	596.9100	508142	28.7
18	597.9145	213789	12.1
19	598.9185	45578	2.6
20	608.9232	8745	0.5
21	618.9218	16616	0.9
22	731.2226	29441	1.7
23	732.2500	80161	4.5
24	733.2565	38463	2.2
25	734.2612	8727	0.5
26	1062.7746	13638	0.8
27	1063.7806	10151	0.6
28	1150.6799	11674	0.7
29	1151.6928	8731	0.5
30	1182.7015	10557	0.6