

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\LR1-83_P1-C-4_01_6195.d
Method lc_qtof_directospos.m
Sample Name LR1-83
Comment Sv: DCM + MeOH + HCOOH
Durán


Acquisition Date 12/15/2022 3:04:42 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

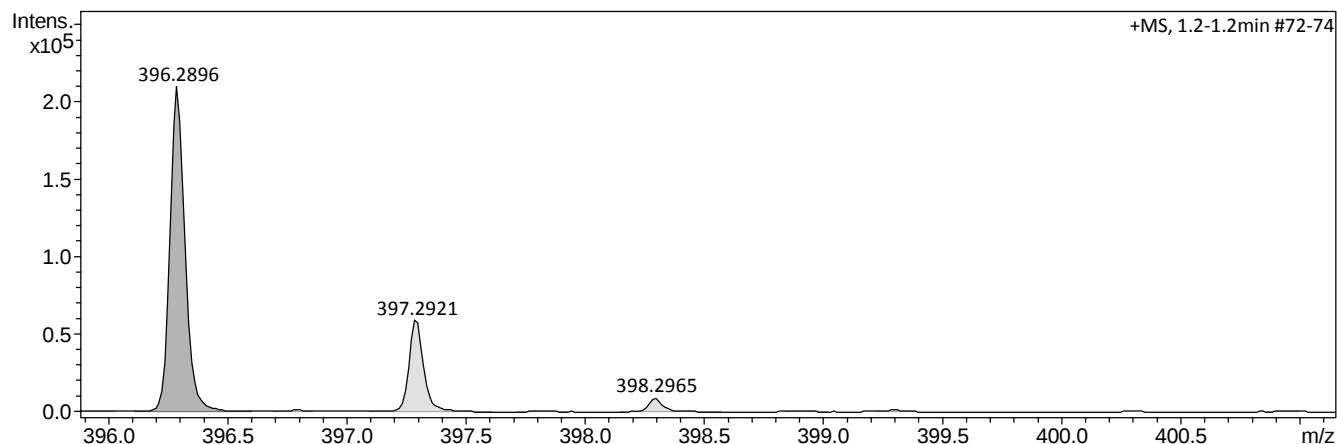

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
396.2896	1	C ₂₆ H ₃₈ NO ₂	396.2897	0.4	5.9	1	100.00	8.5	even	ok