

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\LR2-11_P1-E-8_01_9688.d
 Method lc_ms directos tunelow300924.m
 Sample Name LR2-11
 Comment Sv: MeOH + HCOOH
 Fernando Durán


Acquisition Date 11/11/2024 3:37:10 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

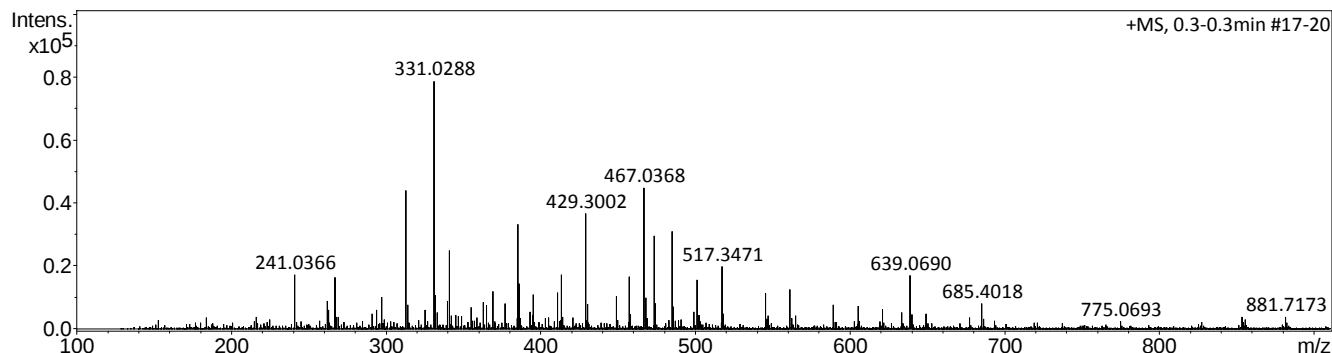

#	m/z	I	I %
1	241.0366	17187	21.9
2	262.1225	8883	11.3
3	267.0133	16439	20.9
4	297.2250	10068	12.8
5	313.0194	43918	55.9
6	331.0288	78596	100.0
7	332.0314	10596	13.5
8	340.0029	8966	11.4
9	341.2523	24858	31.6
10	363.0493	8550	10.9
11	369.2800	11861	15.1
12	385.2747	33122	42.1
13	386.0066	14261	18.1
14	395.1768	10860	13.8
15	411.0487	11494	14.6
16	413.2987	17252	21.9
17	429.0676	8447	10.7
18	429.3002	36541	46.5
19	449.0274	10360	13.2
20	457.3290	16620	21.1
21	467.0368	44630	56.8
22	468.0386	9881	12.6
23	473.3235	29564	37.6
24	474.3270	8152	10.4
25	485.0474	30847	39.2
26	501.3505	15465	19.7
27	517.3471	19713	25.1
28	545.3784	11375	14.5
29	561.3722	12595	16.0
30	639.0690	16942	21.6