

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\LR2-130_P1-C-9_01_10102.d
 Method lc_ms directos tunelow300924.m
 Sample Name LR2-130
 Comment Sv: MeOH + HCOOH
 Fernando Durán

Acquisition Date 9/22/2025 3:28:07 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

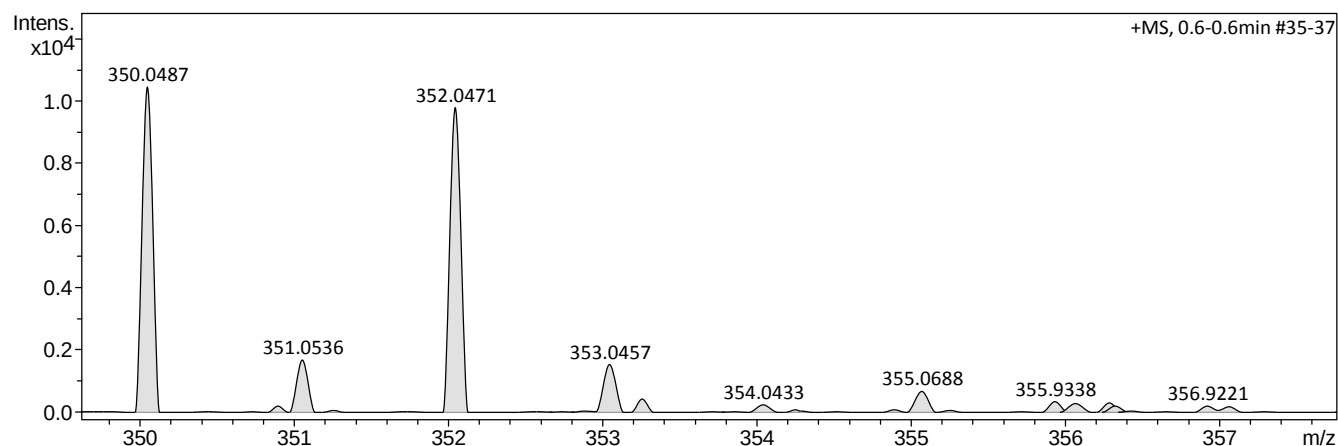

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
350.0487	1	C15H17BrN3O2	350.0499	3.4	28.1	1	100.00	8.5	even	ok