

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\LR2-191-1_P1-C-1_01_10218.d
 Method lc_ms directos tunelow300924.m
 Sample Name LR2-191-1
 Comment Sv: MeOH + HCOOH
 Fernando Durán

Acquisition Date 10/3/2025 12:23:24 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

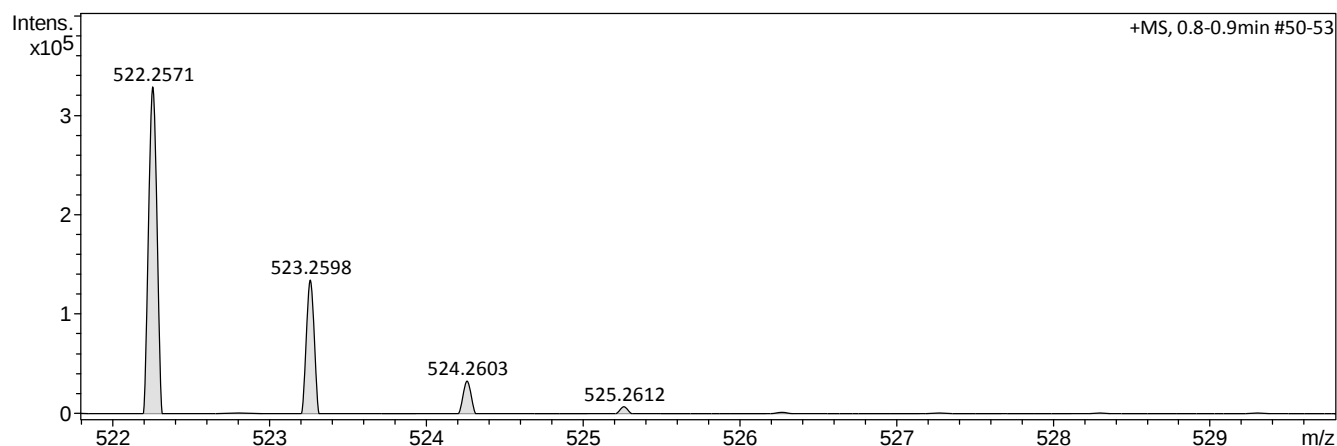

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
522.2571	1	C32H36N3O2Si	522.2571	0.1	10.0	1	100.00	17.5	even	ok