

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-051601_P1-E-5_01_9203.d
 Method lc_qtof_directospos.m
 Sample Name 24-051601
 Comment ZnNAM
 Sv: MeOH
 Evelina Gloria Ferrer

Acquisition Date 5/24/2024 12:10:27 PM

Operator MV
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

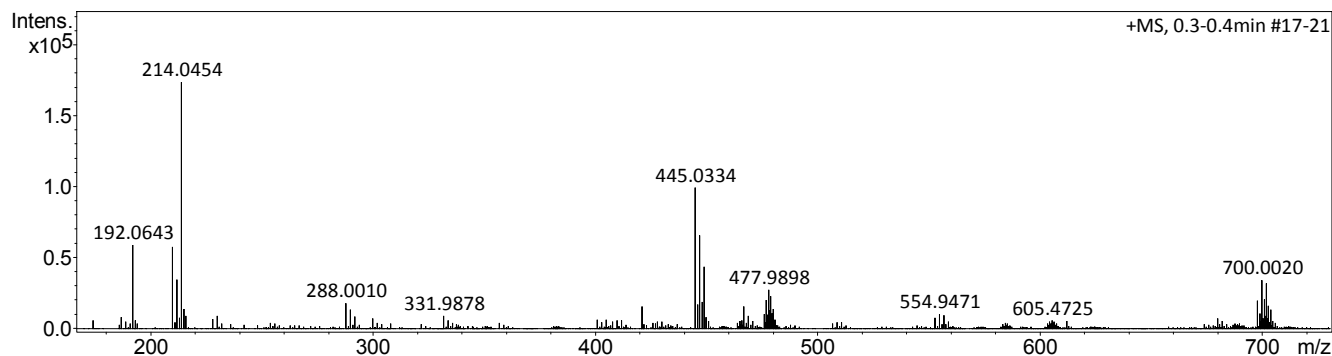

#	m/z	I	I %
1	192.0643	58911	34.1
2	209.9881	57507	33.2
3	211.9847	34649	20.0
4	214.0454	172970	100.0
5	215.0476	14040	8.1
6	288.0010	17856	10.3
7	289.9907	13158	7.6
8	421.0671	15495	9.0
9	445.0334	99314	57.4
10	446.0346	16844	9.7
11	447.0306	65411	37.8
12	448.0321	18702	10.8
13	449.0286	43476	25.1
14	467.0107	15449	8.9
15	475.9905	10231	5.9
16	476.9883	20143	11.6
17	477.4902	9564	5.5
18	477.9898	27136	15.7
19	478.4872	12872	7.4
20	478.9888	22755	13.2
21	479.4876	10744	6.2
22	479.9863	13793	8.0
23	554.9471	10074	5.8
24	698.0046	19665	11.4
25	699.0046	10589	6.1
26	700.0020	33927	19.6
27	701.0033	20422	11.8
28	701.9991	31804	18.4
29	703.0010	15993	9.2
30	703.9962	13259	7.7