

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-051602_P1-E-6_01_9204.d
 Method lc_qtof_directospos.m
 Sample Name 24-051602
 Comment ZnSac
 Sv: MeOH
 Evelina Gloria Ferrer

Acquisition Date 5/24/2024 12:15:34 PM

Operator MV
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

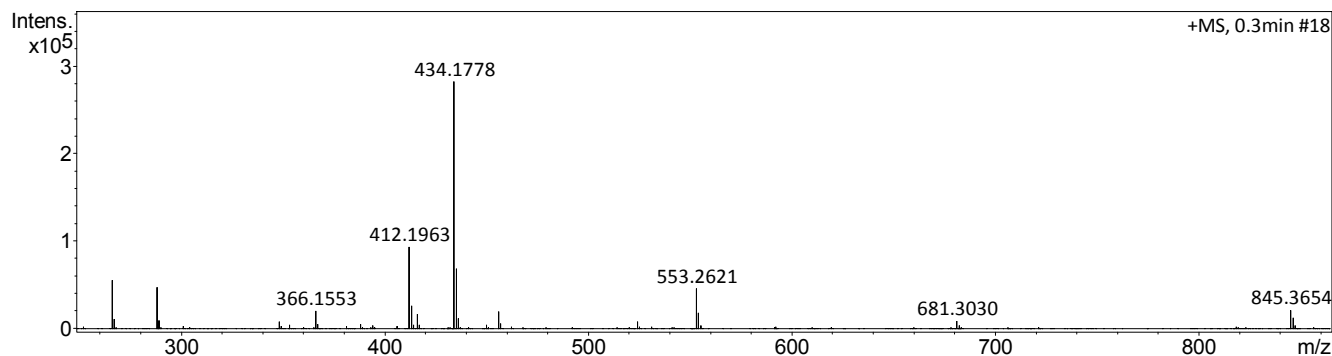

#	m/z	I	I %
1	214.1116	4620	1.6
2	266.1448	55143	19.6
3	267.1481	10898	3.9
4	288.1262	46931	16.7
5	289.1294	9365	3.3
6	348.1439	7528	2.7
7	353.2534	4216	1.5
8	366.1553	19984	7.1
9	367.1593	5185	1.8
10	388.1383	4681	1.7
11	412.1963	92907	33.0
12	413.2018	25859	9.2
13	414.2039	4466	1.6
14	416.1664	16397	5.8
15	417.1724	4028	1.4
16	434.1778	281562	100.0
17	435.1812	68437	24.3
18	436.1815	11456	4.1
19	450.1480	4098	1.5
20	456.1591	19793	7.0
21	457.1624	5991	2.1
22	524.1389	8119	2.9
23	553.2621	45675	16.2
24	554.2637	17821	6.3
25	681.3030	8625	3.1
26	845.3654	21330	7.6
27	846.3695	12249	4.4
28	847.3723	3755	1.3
29	867.3451	6459	2.3
30	889.3228	5755	2.0