

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\MU16_P1-E-2_01_8398.d
 Method lc_qtof_directospos.m
 Sample Name MU16
 Comment Sv: DCM + MeOH + HCOOH
 Garcia Linares

Acquisition Date 12/27/2023 11:27:12 AM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

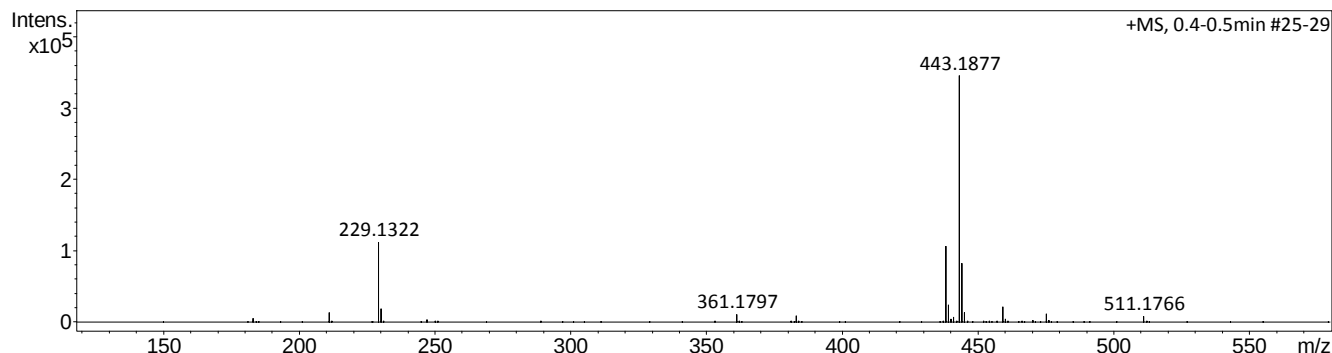

#	m/z	I	I %
1	183.1235	5269	1.5
2	211.1208	13472	3.9
3	229.1322	111318	32.3
4	230.1348	18649	5.4
5	361.1797	10515	3.0
6	383.1627	9077	2.6
7	438.2319	106141	30.8
8	439.2347	23896	6.9
9	440.2351	4320	1.3
10	441.1734	7313	2.1
11	443.1877	344990	100.0
12	444.1896	82278	23.8
13	445.1923	13626	3.9
14	459.1672	21418	6.2
15	460.1704	4917	1.4
16	475.1766	11322	3.3
17	511.1766	8195	2.4
18	858.4318	14276	4.1
19	859.4316	6655	1.9
20	861.3707	7467	2.2
21	862.3725	3528	1.0
22	863.3856	215199	62.4
23	864.3896	101752	29.5
24	865.3930	26576	7.7
25	866.3950	6284	1.8
26	879.3713	13701	4.0
27	880.3743	6407	1.9
28	895.3729	10065	2.9
29	896.3749	5174	1.5
30	931.3758	4087	1.2