

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\MU4_P1-E-1_01_8397.d
 Method lc_qtof_directospos.m
 Sample Name MU4
 Comment Sv: DCM + MeOH + HCOOH
 Garcia Linares

Acquisition Date 12/27/2023 11:22:06 AM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

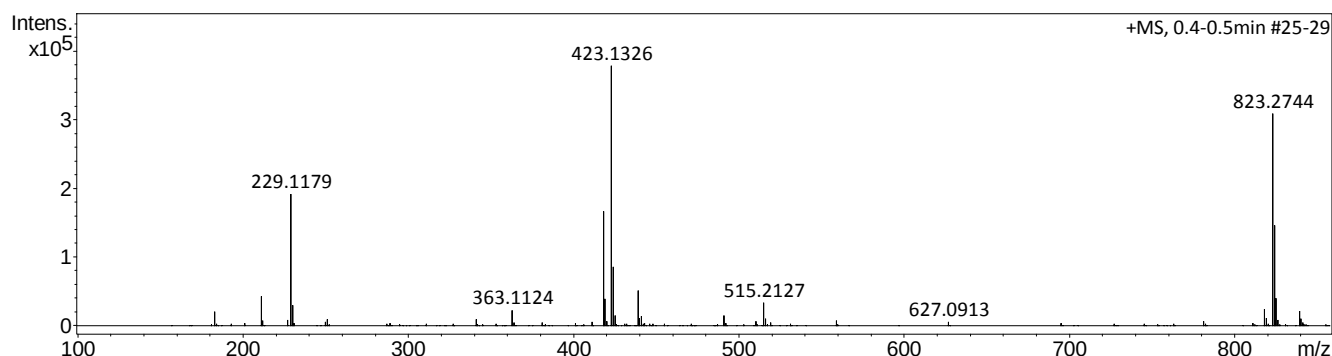

#	m/z	I	I %
1	183.1139	20196	5.3
2	211.1079	43179	11.4
3	212.1112	7486	2.0
4	226.9461	8070	2.1
5	229.1179	191041	50.6
6	230.1201	29972	7.9
7	251.1001	9621	2.5
8	341.1305	9557	2.5
9	363.1124	22463	5.9
10	418.1769	166496	44.1
11	419.1780	39411	10.4
12	423.1326	377606	100.0
13	424.1362	85657	22.7
14	425.1358	14720	3.9
15	439.1083	50962	13.5
16	440.1107	11121	2.9
17	441.1313	13807	3.7
18	491.1199	14935	4.0
19	515.2127	33605	8.9
20	516.2185	9950	2.6
21	559.1026	7431	2.0
22	818.3175	24531	6.5
23	819.3166	10990	2.9
24	823.2744	308722	81.8
25	824.2781	146285	38.7
26	825.2808	40197	10.6
27	826.2760	8192	2.2
28	839.2519	21465	5.7
29	840.2555	10819	2.9
30	891.2535	7023	1.9