

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\STL3_P1-E-3_01_8399.d
 Method lc_qtof_directospos.m
 Sample Name STL3
 Comment Sv: DCM + MeOH + HCOOH
 Garcia Linares

Acquisition Date 12/27/2023 11:32:19 AM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

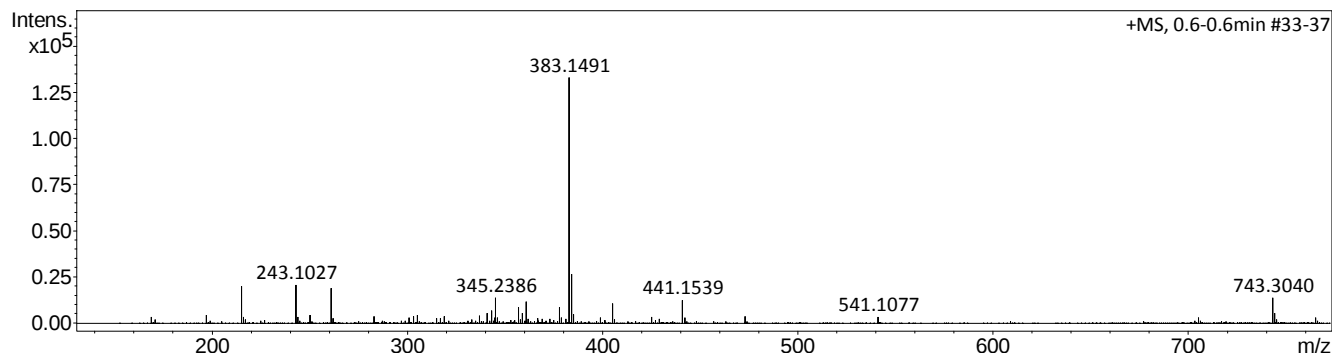

#	m/z	I	I %
1	169.1019	3460	2.6
2	197.0991	4451	3.4
3	215.1081	19956	15.0
4	216.1113	3343	2.5
5	243.1027	20620	15.5
6	244.1065	3254	2.4
7	250.1448	4285	3.2
8	261.1144	18815	14.2
9	283.0956	3786	2.8
10	303.2319	3739	2.8
11	305.2463	4400	3.3
12	319.2243	3787	2.9
13	337.0712	4032	3.0
14	341.2093	5576	4.2
15	343.2162	6819	5.1
16	345.2386	13834	10.4
17	357.2058	8402	6.3
18	359.2177	5378	4.0
19	361.1709	11578	8.7
20	378.1936	8693	6.5
21	383.1491	132853	100.0
22	384.1529	26667	20.1
23	385.1571	4828	3.6
24	405.1325	10792	8.1
25	425.1596	3228	2.4
26	441.1539	12378	9.3
27	473.1175	3593	2.7
28	541.1077	3284	2.5
29	743.3040	13782	10.4
30	744.3071	5388	4.1