

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\STL4_P1-E-4_01_8400.d
 Method lc_qtof_directospos.m
 Sample Name STL4
 Comment Sv: DCM + MeOH + HCOOH
 Garcia Linares

Acquisition Date 12/27/2023 11:37:28 AM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

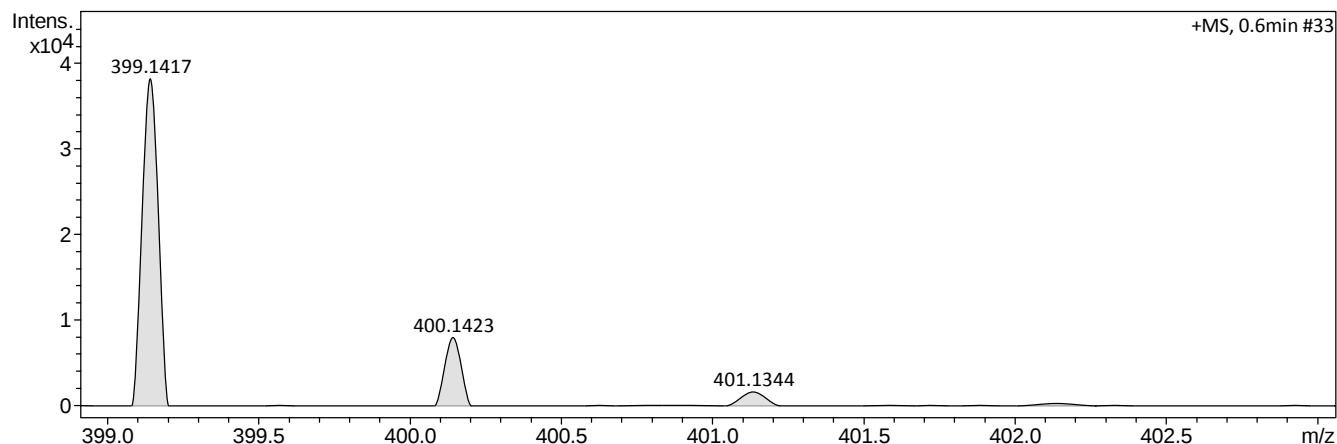

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
399.1417	1	C20H24NaO7	399.1414	-0.6	23.1	1	100.00	8.5	even	ok