

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\compZ_P1-E-5_01_8401.d
 Method lc_qtof_directospos.m
 Sample Name compZ
 Comment Sv: DCM + MeOH + HCOOH
 Garcia Linares

Acquisition Date 12/27/2023 11:42:37 AM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

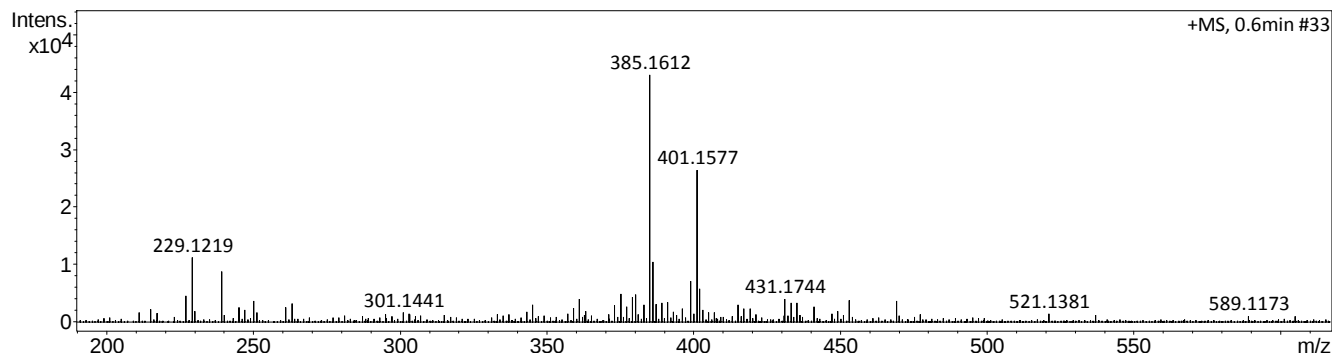

#	m/z	I	I %
1	226.9516	4544	10.6
2	229.1219	11234	26.2
3	239.1603	8719	20.3
4	250.1420	3687	8.6
5	263.1260	3272	7.6
6	345.2209	2948	6.9
7	361.0973	3996	9.3
8	361.1885	3459	8.1
9	373.1948	2846	6.6
10	375.1961	4913	11.5
11	379.1779	4380	10.2
12	380.2022	4771	11.1
13	383.0841	3006	7.0
14	385.1612	42902	100.0
15	386.1648	10440	24.3
16	387.1629	3141	7.3
17	389.1905	3283	7.7
18	391.2022	3482	8.1
19	399.1429	7091	16.5
20	401.1577	26383	61.5
21	402.1585	5769	13.4
22	415.1586	3035	7.1
23	431.1744	4024	9.4
24	433.2104	3319	7.7
25	435.2287	3361	7.8
26	453.1511	3750	8.7
27	469.1481	3672	8.6
28	747.3308	5112	11.9
29	761.3018	2776	6.5
30	763.3228	5437	12.7