

# Qualitative Compound Report

## Analysis Info

Analysis Name D:\Data\ggc\22-111003\_P1-C-3\_01\_5987.d  
Method lc\_qtof\_directospos.m  
Sample Name 22-111003  
Comment iBuSG  
Sv: MeOH + HCOOH  
Gavernet


Acquisition Date 11/14/2022 1:21:16 PM

Operator ELB  
Instrument micrOTOF-Q II



## Acquisition Parameter

|             |            |                       |           |                  |           |
|-------------|------------|-----------------------|-----------|------------------|-----------|
| Source Type | ESI        | Ion Polarity          | Positive  | Set Nebulizer    | 3.5 Bar   |
| Focus       | Not active | Set Capillary         | 4000 V    | Set Dry Heater   | 200 °C    |
| Scan Begin  | 100 m/z    | Set End Plate Offset  | -500 V    | Set Dry Gas      | 7.0 l/min |
| Scan End    | 1500 m/z   | Set Collision Cell RF | 300.0 Vpp | Set Divert Valve | Source    |

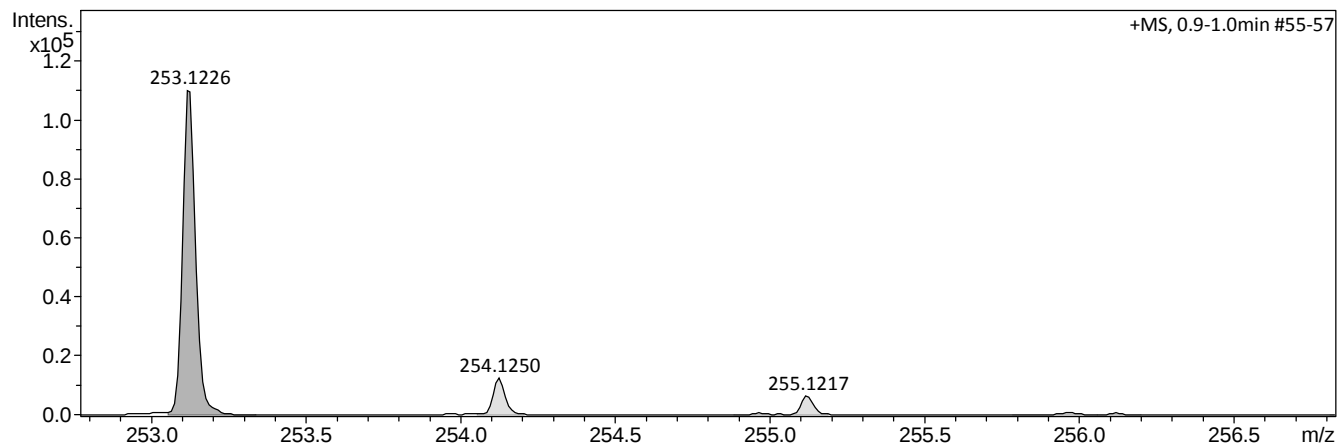

| Meas. m/z | # | Ion Formula | m/z      | err [ppm] | mSigma | # mSigma | Score  | rdb | e <sup>-</sup> Conf | N-Rule |
|-----------|---|-------------|----------|-----------|--------|----------|--------|-----|---------------------|--------|
| 253.1226  | 1 | C9H21N2O4S  | 253.1217 | -3.7      | 2.0    | 1        | 100.00 | 0.5 | even                | ok     |