

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-110802_P1-E-1_01_9736.d
 Method lc-qtof directos tune high 151124 neg.m
 Sample Name 24-110802
 Comment Muestra 1
 Sv: MeOH + Agua
 Iribarren

Acquisition Date 11/15/2024 4:38:37 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	400 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	3100 m/z	Set Collision Cell RF	600.0 Vpp	Set Divert Valve	Source

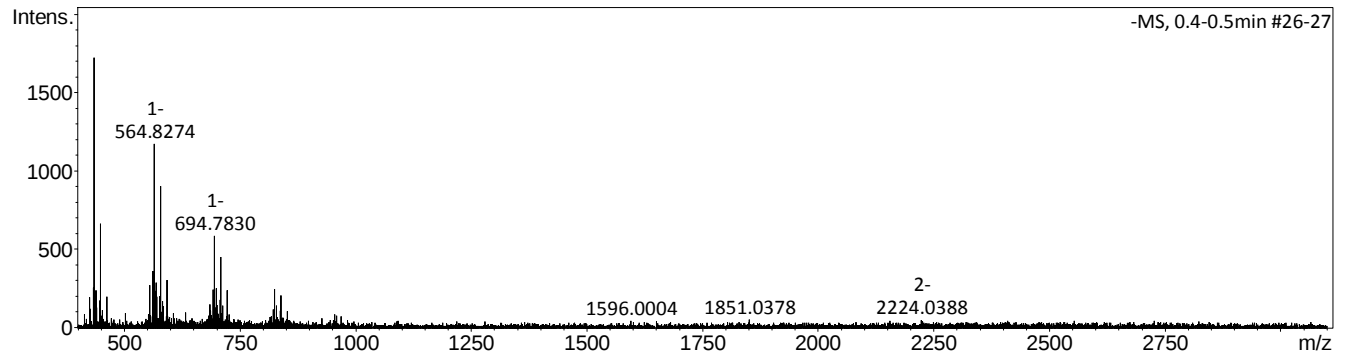

#	m/z	I	I %
1	424.8431	195	11.3
2	432.8893	256	14.9
3	434.8664	1718	100.0
4	435.8670	142	8.3
5	438.8543	242	14.1
6	446.9030	173	10.1
7	448.8847	663	38.6
8	462.9024	198	11.5
9	554.8036	274	16.0
10	562.8433	362	21.1
11	564.8274	1169	68.1
12	565.8318	177	10.3
13	566.8323	234	13.7
14	568.8163	287	16.7
15	570.7977	201	11.7
16	576.8632	203	11.8
17	578.8391	903	52.6
18	582.8330	170	9.9
19	592.8601	306	17.8
20	684.7592	151	8.8
21	692.7977	245	14.2
22	694.7830	586	34.1
23	698.7745	250	14.6
24	700.7689	147	8.6
25	706.8119	178	10.4
26	708.8031	451	26.3
27	712.8034	144	8.4
28	722.8205	240	13.9
29	824.7369	247	14.4
30	838.7560	208	12.1