

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-110803_P1-E-2_01_9737.d
 Method lc-qtof directos tune high 151124 neg.m
 Sample Name 24-110803
 Comment Muestra 2
 Sv: MeOH + Agua
 Iribarren


Acquisition Date 11/15/2024 4:43:45 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	400 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	3100 m/z	Set Collision Cell RF	600.0 Vpp	Set Divert Valve	Source

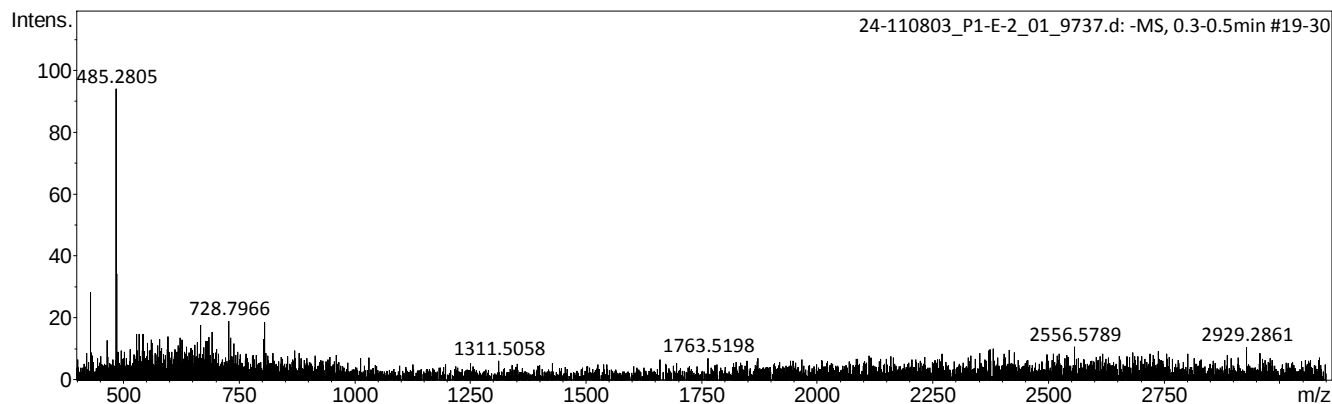

#	m/z	I	I %
1	429.1911	28	30.0
2	465.1947	13	13.7
3	485.2805	94	100.0
4	486.2891	34	36.3
5	528.8559	15	15.8
6	535.2283	15	15.8
7	543.2184	15	15.8
8	552.7744	12	12.7
9	560.8314	13	13.7
10	562.8777	12	12.6
11	574.8417	11	11.7
12	578.8927	13	14.1
13	596.8374	11	12.1
14	597.2993	14	14.9
15	618.8443	11	11.7
16	622.8523	14	14.5
17	626.8105	13	13.7
18	654.8018	11	12.0
19	660.8574	12	12.8
20	666.7945	18	18.9
21	677.8207	12	13.3
22	680.8021	13	13.4
23	684.8691	14	14.8
24	692.8515	16	16.5
25	728.7966	19	20.2
26	732.8065	14	14.5
27	738.7804	12	12.5
28	804.7609	13	14.0
29	805.9651	19	19.8
30	2556.5789	11	11.4